

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019273.D
 Acq On : 05 Nov 2020 13:08
 Operator : SY/MD
 Sample : L4543-16ME
 Misc : 5.70g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG474ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC: VV0192273.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	62	69	90	rVB	217018	268749	14.48%	2.008%
2	1.573	143	150	164	rBV	175351	280825	15.13%	2.099%
3	2.100	303	314	325	rBV	458348	665857	35.87%	4.976%
4	2.344	387	390	391	rBV	310	137	0.01%	0.001%
5	2.434	416	418	420	rBV	375	213	0.01%	0.002%
6	2.627	466	478	491	rBV3	5469	11810	0.64%	0.088%
7	2.753	515	517	519	rBV2	276	120	0.01%	0.001%
8	2.920	567	569	574	rBV2	394	300	0.02%	0.002%
9	3.042	605	607	609	rVB	359	117	0.01%	0.001%
10	3.145	635	639	644	rBV	382	419	0.02%	0.003%
11	3.306	685	689	691	rBV2	315	220	0.01%	0.002%
12	3.376	708	711	712	rBV	296	161	0.01%	0.001%
13	3.425	724	726	728	rBV	187	106	0.01%	0.001%
14	3.473	739	741	743	rVB	211	72	0.00%	0.001%
15	3.518	752	755	759	rBV	310	197	0.01%	0.001%
16	3.682	802	806	812	rVB2	454	391	0.02%	0.003%
17	3.714	812	816	821	rBV2	384	466	0.03%	0.003%
18	3.762	826	831	835	rBV	246	275	0.01%	0.002%
19	3.804	841	844	851	rBV2	271	274	0.01%	0.002%
20	3.839	851	855	859	rBV	265	255	0.01%	0.002%
21	3.910	866	877	924	rBV	82249	329691	17.76%	2.464%
22	4.363	1003	1018	1056	rVB	285410	735614	39.63%	5.498%
23	4.582	1084	1086	1089	rVB3	339	140	0.01%	0.001%
24	4.611	1089	1095	1096	rBV2	397	357	0.02%	0.003%
25	4.769	1139	1144	1149	rBV2	367	473	0.03%	0.004%
26	4.833	1160	1164	1166	rBV2	421	334	0.02%	0.002%
27	4.878	1176	1178	1181	rBV	216	123	0.01%	0.001%
28	5.061	1217	1235	1273	rBV2	737956	1856132	100.00%	13.872%
29	5.357	1322	1327	1333	rBV6	1118	1605	0.09%	0.012%
30	5.498	1368	1371	1374	rBV	230	198	0.01%	0.001%
31	5.563	1389	1391	1393	rBV	181	78	0.00%	0.001%
32	5.588	1396	1399	1400	rBV	178	113	0.01%	0.001%
33	5.634	1400	1413	1448	rBV	398469	816306	43.98%	6.101%
34	5.923	1491	1503	1523	rBV3	20138	43788	2.36%	0.327%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019273.D
 Acq On : 05 Nov 2020 13:08
 Operator : SY/MD
 Sample : L4543-16ME
 Misc : 5.70µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG474ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	6.003	1525	1528	1531	rBV3	987	906	0.05%	0.007%
36	6.087	1541	1554	1580	rBV	394392	827976	44.61%	6.188%
37	6.347	1632	1635	1637	rBV	422	311	0.02%	0.002%
38	6.656	1726	1731	1740	rBV4	1099	1883	0.10%	0.014%
39	6.775	1767	1768	1772	rVB2	456	176	0.01%	0.001%
40	6.794	1772	1774	1778	rVB	321	204	0.01%	0.002%
41	6.814	1778	1780	1784	rBV	226	166	0.01%	0.001%
42	6.839	1784	1788	1791	rBV2	220	204	0.01%	0.002%
43	6.913	1809	1811	1812	rBV	202	113	0.01%	0.001%
44	7.003	1827	1839	1865	rBV	225786	444226	23.93%	3.320%
45	7.283	1924	1926	1928	rBV	323	174	0.01%	0.001%
46	7.331	1928	1941	1960	rBV	864609	1517881	81.78%	11.344%
47	7.592	2020	2022	2025	rVB2	495	257	0.01%	0.002%
48	7.640	2025	2037	2067	rBV	156551	315470	17.00%	2.358%
49	7.881	2110	2112	2114	rBV3	245	127	0.01%	0.001%
50	7.994	2136	2147	2166	rVB2	71398	122112	6.58%	0.913%
51	8.132	2173	2190	2227	rBV	271788	826081	44.51%	6.174%
52	8.453	2284	2290	2297	rBV4	743	1289	0.07%	0.010%
53	8.637	2344	2347	2348	rBV	410	195	0.01%	0.001%
54	8.785	2389	2393	2395	rBV	348	291	0.02%	0.002%
55	8.871	2408	2420	2449	rBV	577386	1032304	55.62%	7.715%
56	9.132	2497	2501	2504	rVB2	291	206	0.01%	0.002%
57	9.167	2506	2512	2516	rBV6	914	1101	0.06%	0.008%
58	9.238	2531	2534	2538	rBV	373	318	0.02%	0.002%
59	9.283	2546	2548	2552	rVB2	414	273	0.01%	0.002%
60	9.302	2552	2554	2555	rBV2	128	58	0.00%	0.000%
61	9.315	2555	2558	2562	rBV	373	321	0.02%	0.002%
62	9.395	2580	2583	2585	rBV	295	216	0.01%	0.002%
63	9.566	2634	2636	2638	rBV	302	185	0.01%	0.001%
64	9.842	2719	2722	2724	rBV2	206	170	0.01%	0.001%
65	9.903	2737	2741	2744	rBV	219	186	0.01%	0.001%
66	10.042	2781	2784	2787	rBV	364	332	0.02%	0.002%
67	10.074	2791	2794	2796	rBV	254	169	0.01%	0.001%
68	10.148	2809	2817	2825	rBV6	2542	4327	0.23%	0.032%
69	10.241	2833	2846	2866	rBV	465862	790764	42.60%	5.910%
70	10.395	2891	2894	2896	rBV2	703	491	0.03%	0.004%
71	10.479	2916	2920	2922	rBV2	298	252	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019273.D
 Acq On : 05 Nov 2020 13:08
 Operator : SY/MD
 Sample : L4543-16ME
 Misc : 5.70g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG474ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.547	2939	2941	2943	rBV	252	171	0.01%	0.001%
73	10.592	2953	2955	2961	rBV5	736	695	0.04%	0.005%
74	10.727	2991	2997	3004	rBV2	363	631	0.03%	0.005%
75	11.273	3155	3167	3193	rBV	670792	1027450	55.35%	7.679%
76	11.402	3204	3207	3209	rBV3	995	745	0.04%	0.006%
77	11.569	3257	3259	3262	rBV2	281	187	0.01%	0.001%
78	11.649	3271	3284	3306	rBV	920494	1438121	77.48%	10.748%
79	11.845	3341	3345	3347	rBV	350	269	0.01%	0.002%
80	11.993	3385	3391	3393	rBV2	433	390	0.02%	0.003%
81	12.177	3445	3448	3452	rBV	265	198	0.01%	0.001%
82	12.463	3533	3537	3540	rBV2	358	376	0.02%	0.003%
83	12.617	3582	3585	3586	rBV2	270	151	0.01%	0.001%
84	13.292	3792	3795	3797	rBV2	417	231	0.01%	0.002%
85	13.321	3802	3804	3807	rBV	327	160	0.01%	0.001%
86	13.537	3869	3871	3874	rBV2	278	153	0.01%	0.001%
87	13.646	3903	3905	3906	rBV2	353	160	0.01%	0.001%
88	13.887	3976	3980	3982	rBV2	417	384	0.02%	0.003%
89	14.061	4025	4034	4042	rBV3	1268	2254	0.12%	0.017%
90	14.543	4181	4184	4186	rBV2	461	369	0.02%	0.003%


Sum of corrected areas: 13380726

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110720\
Data File : VV019273.D
Acq On : 05 Nov 2020 13:08
Operator : SY/MD
Sample : L4543-16ME
Misc : 5.70µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG474ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

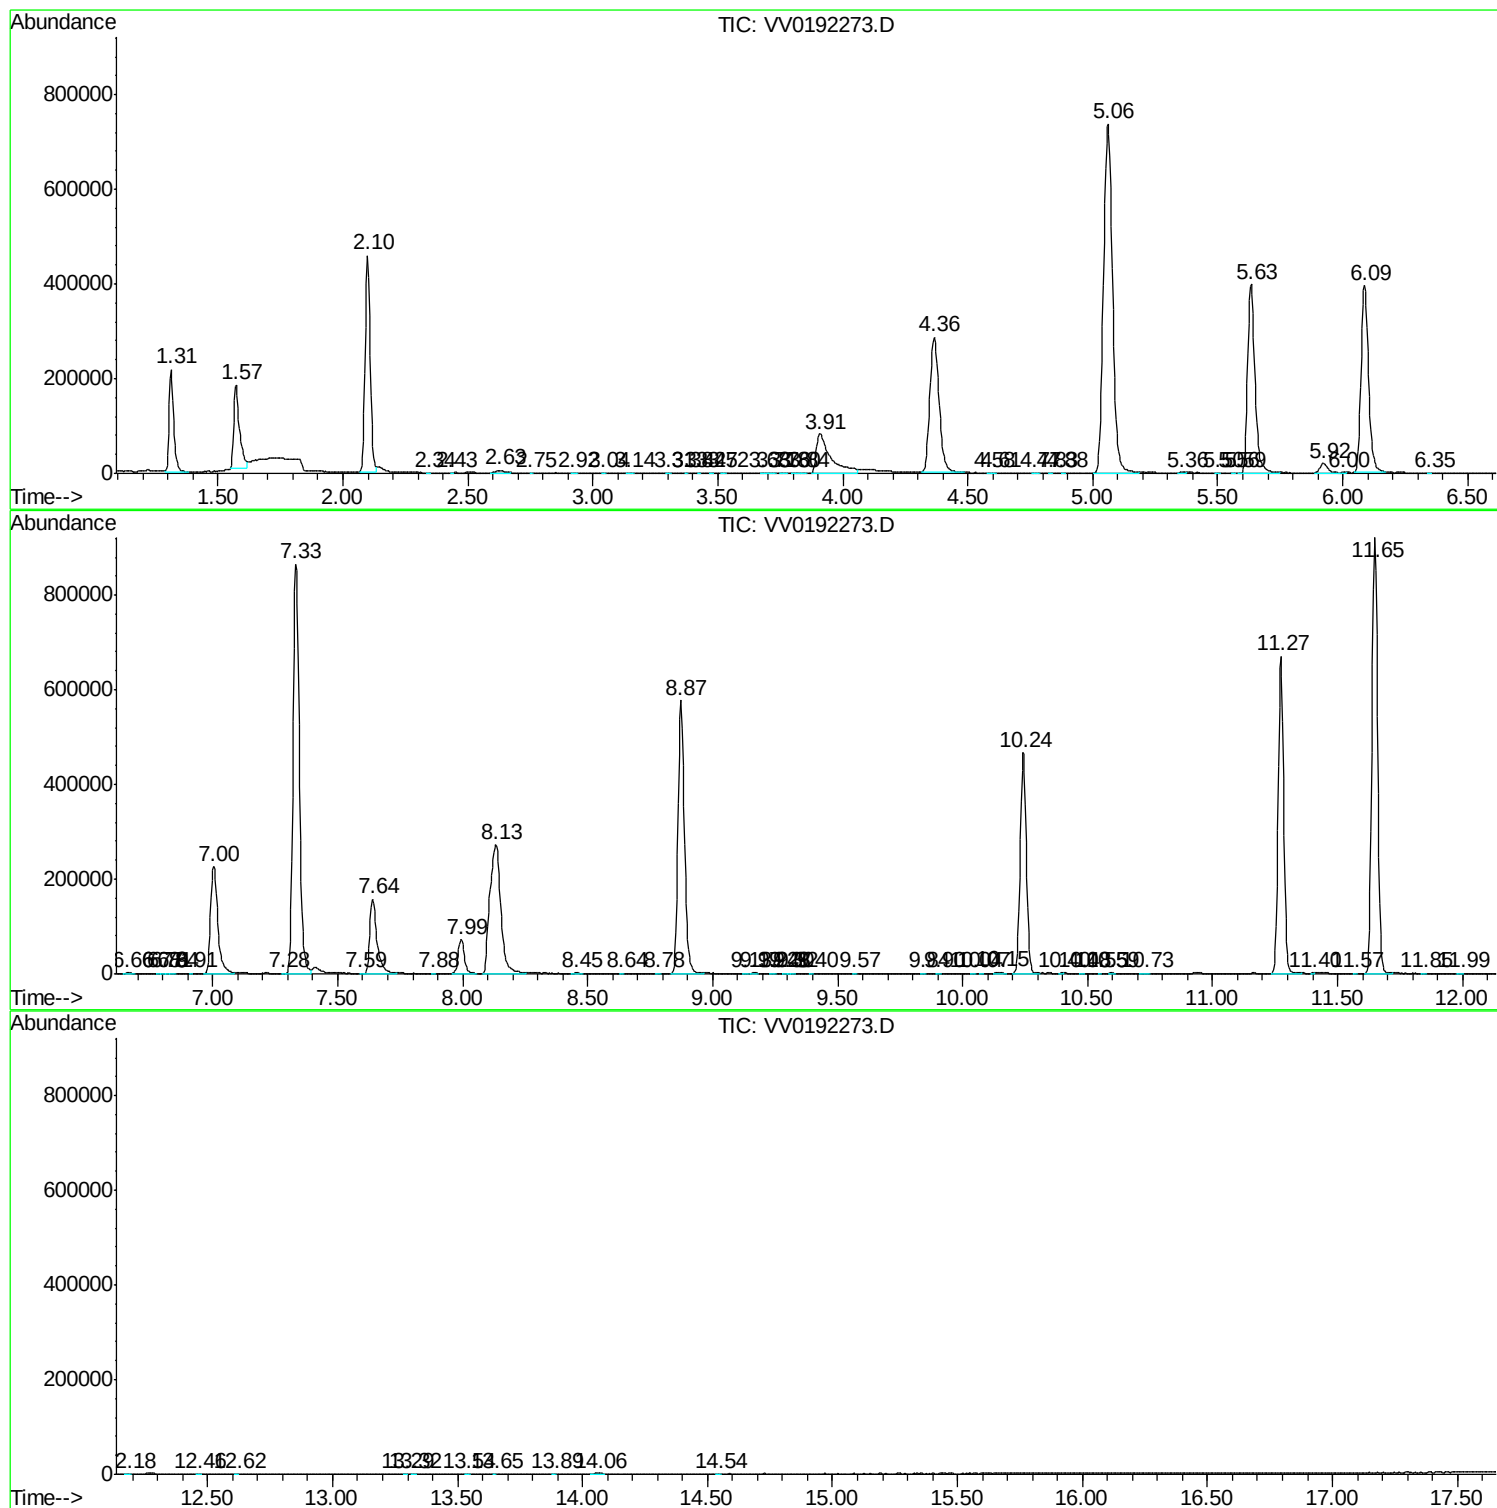

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110720\
Data File : VV019273.D
Acq On : 05 Nov 2020 13:08
Operator : SY/MD
Sample : L4543-16ME
Misc : 5.70g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG474ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110720\
Data File : VV019273.D
Acq On : 05 Nov 2020 13:08
Operator : SY/MD
Sample : L4543-16ME
Misc : 5.70g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG474ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc