


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV110720\
 Data File : VV019267.D
 Acq On : 05 Nov 2020 09:15
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Mon Nov 09 02:16:03 2020

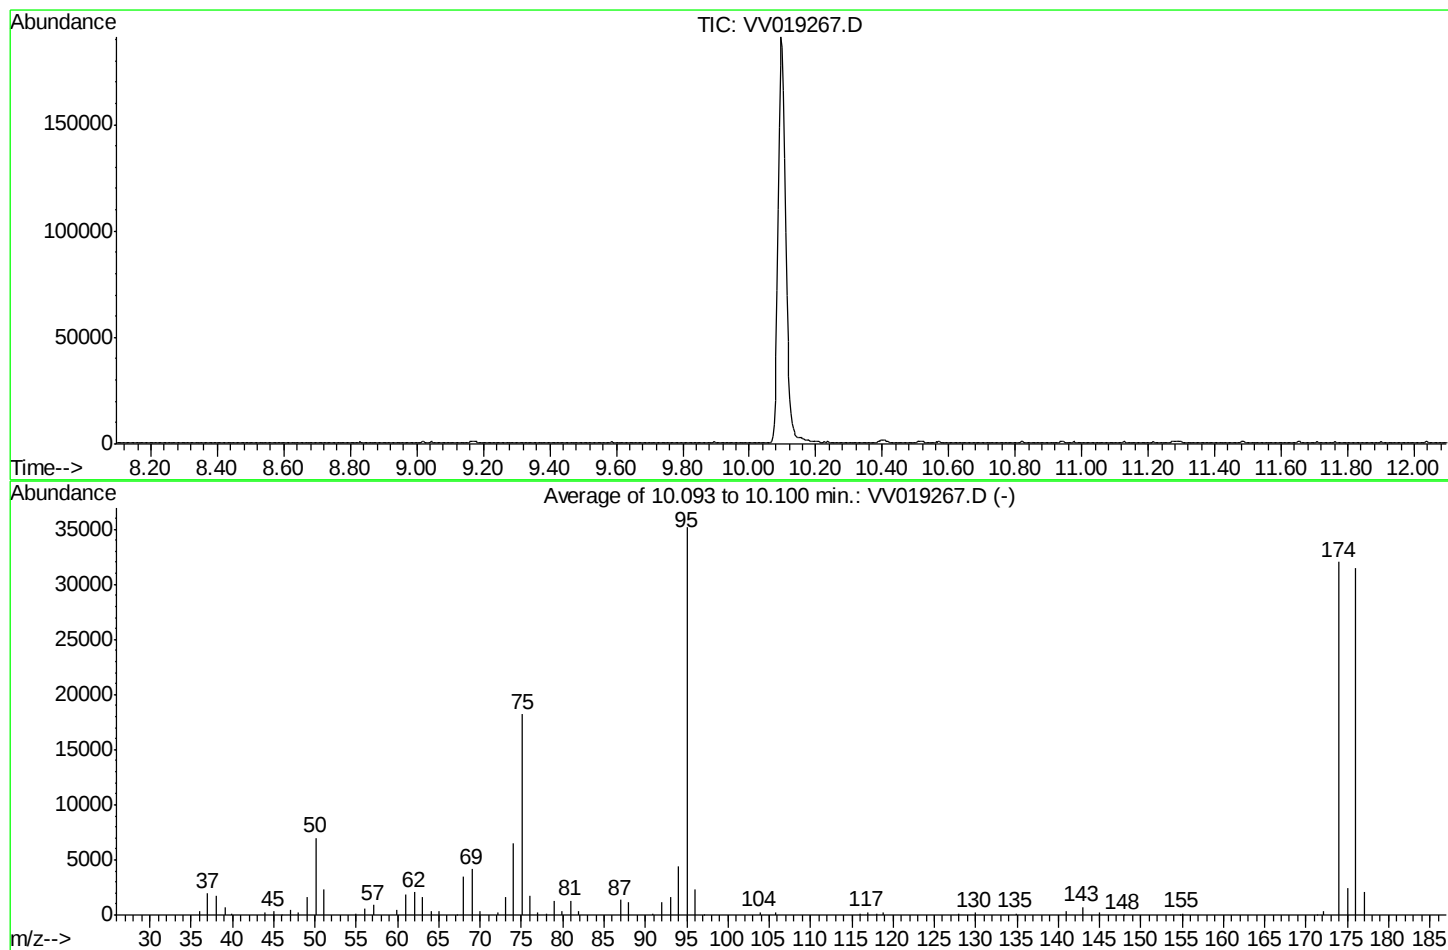

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	6996	PASS
75	95	30	80	51.8	18202	PASS
95	95	100	100	100.0	35168	PASS
96	95	5	9	6.7	2339	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.0	31997	PASS
175	174	5	9	7.5	2409	PASS
176	174	95	101	98.3	31448	PASS
177	176	5	9	6.6	2085	PASS

m/z	Abundance
36.00	361.0
37.00	1974.0
38.00	1676.0
39.10	781.0
40.00	127.0
44.00	841.0
45.00	378.0
46.00	106.0
47.00	460.0
47.90	258.0
49.10	1573.0
50.00	6882.0
51.10	2171.0
56.00	635.0
57.00	856.0
59.90	429.0
61.00	1792.0
62.00	1950.0
63.00	1655.0
64.00	290.0
65.00	356.0
68.00	3601.0
69.00	3868.0
70.00	375.0
72.10	275.0
73.00	1598.0
74.00	6311.0
75.10	17552.0
76.00	1624.0
76.90	239.0
77.90	131.0
79.00	1335.0
79.90	348.0
81.00	1289.0
82.00	352.0
87.00	1268.0
88.00	1090.0
90.90	151.0
92.00	1238.0
93.00	1574.0
94.00	4121.0
95.00	34368.0
96.00	2268.0
97.10	111.0
103.90	208.0
105.90	198.0
116.90	222.0
118.00	158.0
118.90	208.0
127.90	155.0
130.00	175.0
134.90	117.0
140.90	375.0
142.90	646.0
144.90	226.0
154.70	132.0
155.00	135.0
172.10	385.0
174.00	30192.0
175.00	2293.0
176.00	29544.0
177.00	2063.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	398.0
37.00	1987.0
38.00	1772.0
39.10	763.0
40.00	117.0
44.00	862.0
45.00	355.0
47.00	450.0
48.00	215.0
49.10	1619.0
50.10	7180.0
51.00	2432.0
55.00	115.0
56.00	636.0
57.10	923.0
59.90	496.0
61.00	1933.0
62.00	2144.0
63.00	1753.0
64.10	304.0
65.00	392.0
68.00	3572.0
69.00	4309.0
70.00	402.0
72.10	270.0
73.00	1670.0
74.10	6653.0
75.10	18832.0
76.00	1807.0
76.90	223.0
78.00	132.0
78.90	1353.0
79.90	358.0
80.90	1380.0
82.00	374.0
87.00	1434.0
88.00	1161.0
91.00	151.0
92.00	1220.0
93.00	1682.0
94.00	4620.0
95.10	36280.0
96.10	2400.0
103.80	253.0
105.90	222.0
116.00	109.0
116.90	272.0
118.00	154.0
118.90	238.0
128.00	160.0
129.90	217.0
134.80	136.0
140.90	400.0
142.90	751.0
144.90	246.0
155.00	160.0
171.30	118.0
172.10	412.0
174.00	33024.0
175.00	2457.0
176.00	32560.0
177.00	2125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	366.0
37.00	1843.0
38.10	1657.0
39.10	667.0
39.90	115.0
44.00	892.0
45.00	290.0
46.90	415.0
48.10	202.0
49.10	1636.0
50.00	6926.0
51.00	2325.0
55.00	144.0
56.00	587.0
57.10	958.0
60.00	501.0
61.00	1948.0
62.00	2163.0
63.00	1629.0
64.10	305.0
65.10	420.0
67.10	110.0
68.00	3306.0
69.00	4261.0
70.00	353.0
72.10	240.0
73.10	1597.0
74.10	6393.0
75.10	18224.0
76.00	1835.0
76.90	183.0
78.10	159.0
78.90	1279.0
79.90	364.0
80.90	1334.0
81.90	317.0
87.00	1446.0
88.00	1189.0
91.00	152.0
91.90	1081.0
93.00	1602.0
94.00	4608.0
95.10	34856.0
96.10	2349.0
103.80	251.0
105.80	213.0
116.00	112.0
116.90	287.0
117.90	138.0
118.80	252.0
128.00	162.0
129.90	244.0
134.90	116.0
140.90	384.0
142.90	747.0
145.00	238.0
147.90	143.0
155.00	129.0
172.00	414.0
174.00	32776.0
175.00	2477.0
176.00	32240.0
177.00	2068.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
44.00	682.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89