

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032862.D
 Acq On : 07 Nov 2023 12:03
 Operator : SY/MD
 Sample : VV1107WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 08 01:38:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	340828	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	385067	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	177626	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	145827	44.984	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.960%
7) Chloroethane-d5	1.532	69	129186	47.649	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.300%
11) 1,1-Dichloroethene-d2	2.059	65	63090	47.118	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.240%
21) 2-Butanone-d5	3.783	46	134600	95.725	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.730%
24) Chloroform-d	4.249	84	253116	48.918	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.840%
26) 1,2-Dichloroethane-d4	4.940	65	167451	52.070	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.140%
32) Benzene-d6	4.960	84	492625	49.757	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.520%
36) 1,2-Dichloropropane-d6	5.989	67	164579	54.716	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	109.440%
41) Toluene-d8	7.243	98	479551	49.191	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.380%
43) trans-1,3-Dichloroprop...	7.551	79	77418	49.420	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.840%
47) 2-Hexanone-d5	8.024	63	97279	88.589	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.590%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	221552	48.539	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.080%
66) 1,2-Dichlorobenzene-d4	11.561	152	190145	55.550	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.100%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.551	75	4088	0.979	ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032862.D
Acq On : 07 Nov 2023 12:03
Operator : SY/MD
Sample : VV1107WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 08 01:38:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

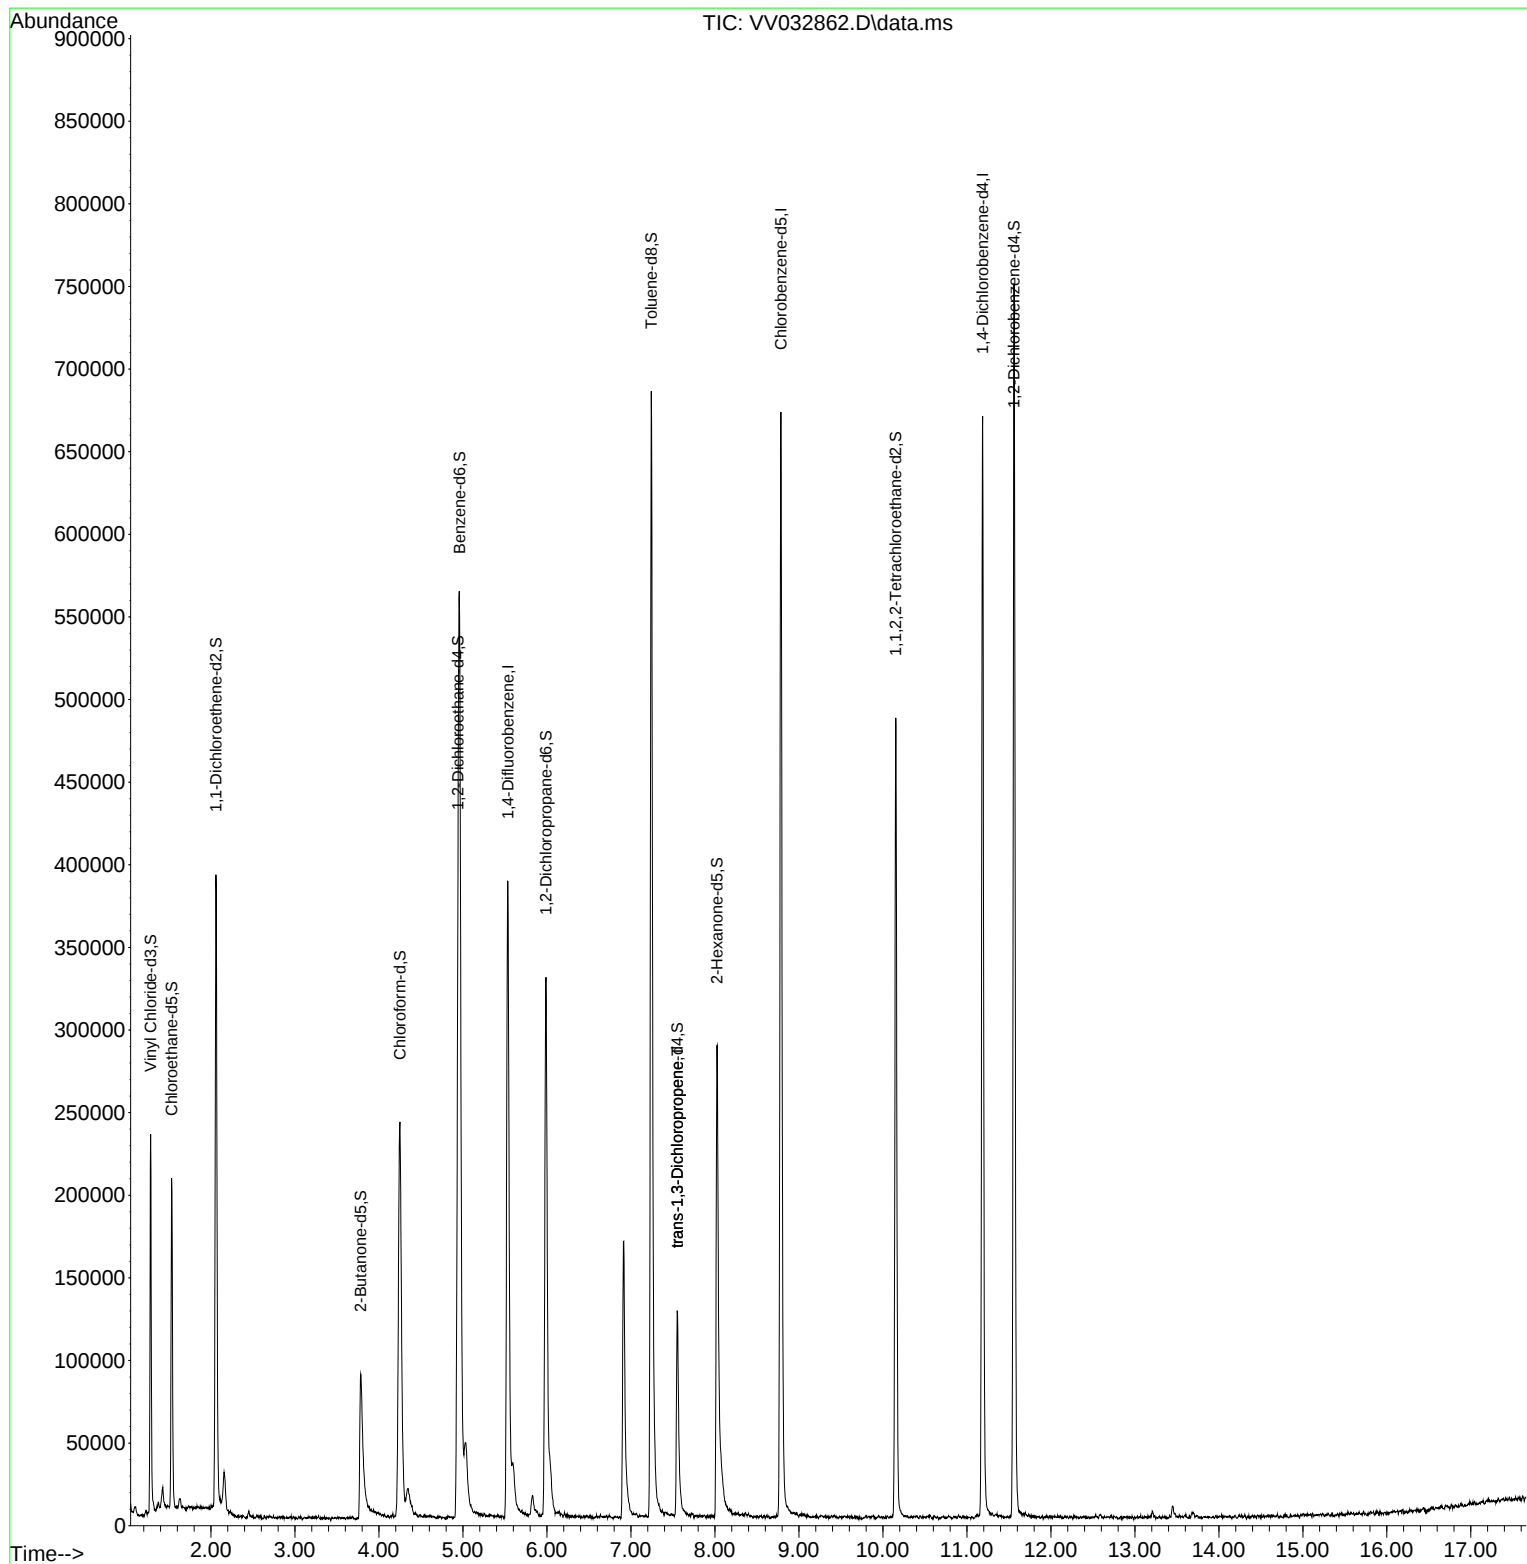

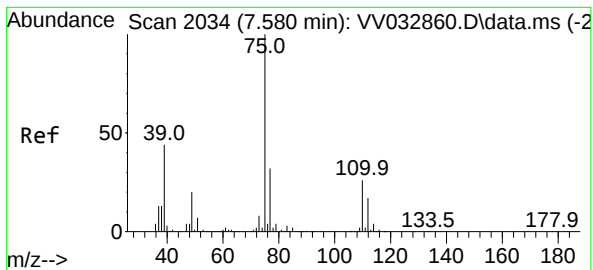

#44
 trans-1,3-Dichloropropene
 Concen: 0.979 ug/L
 RT: 7.551 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: VV032862.D
 Acq: 07 Nov 2023 12:03

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4088
 Ion Ratio Lower Upper
 75 100
 77 52.6 22.0 40.8#

