

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032869.D
 Acq On : 07 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05226-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 08 01:40:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	337949	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	376865	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	167014	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	158174	49.209	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.420%	
7) Chloroethane-d5	1.532	69	137395	51.108	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.220%	
11) 1,1-Dichloroethene-d2	2.060	65	67999	51.217	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	102.440%	
21) 2-Butanone-d5	3.786	46	145210	104.151	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	104.150%	
24) Chloroform-d	4.252	84	257693	50.226	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.460%	
26) 1,2-Dichloroethane-d4	4.944	65	165498	51.901	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.800%	
32) Benzene-d6	4.963	84	507840	52.410	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	104.820%	
36) 1,2-Dichloropropane-d6	5.992	67	153343	52.090	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	104.180%	
41) Toluene-d8	7.246	98	484979	50.831	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.660%	
43) trans-1,3-Dichloroprop...	7.554	79	73882	48.189	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.380%	
47) 2-Hexanone-d5	8.027	63	106113	98.737	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.740%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	227411	50.907	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	101.820%	
66) 1,2-Dichlorobenzene-d4	11.564	152	195422	60.719	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	121.440%#	
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.558	75	4137	1.012	ug/L	# 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032869.D
Acq On : 07 Nov 2023 15:04
Operator : SY/MD
Sample : 05226-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 08 01:40:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

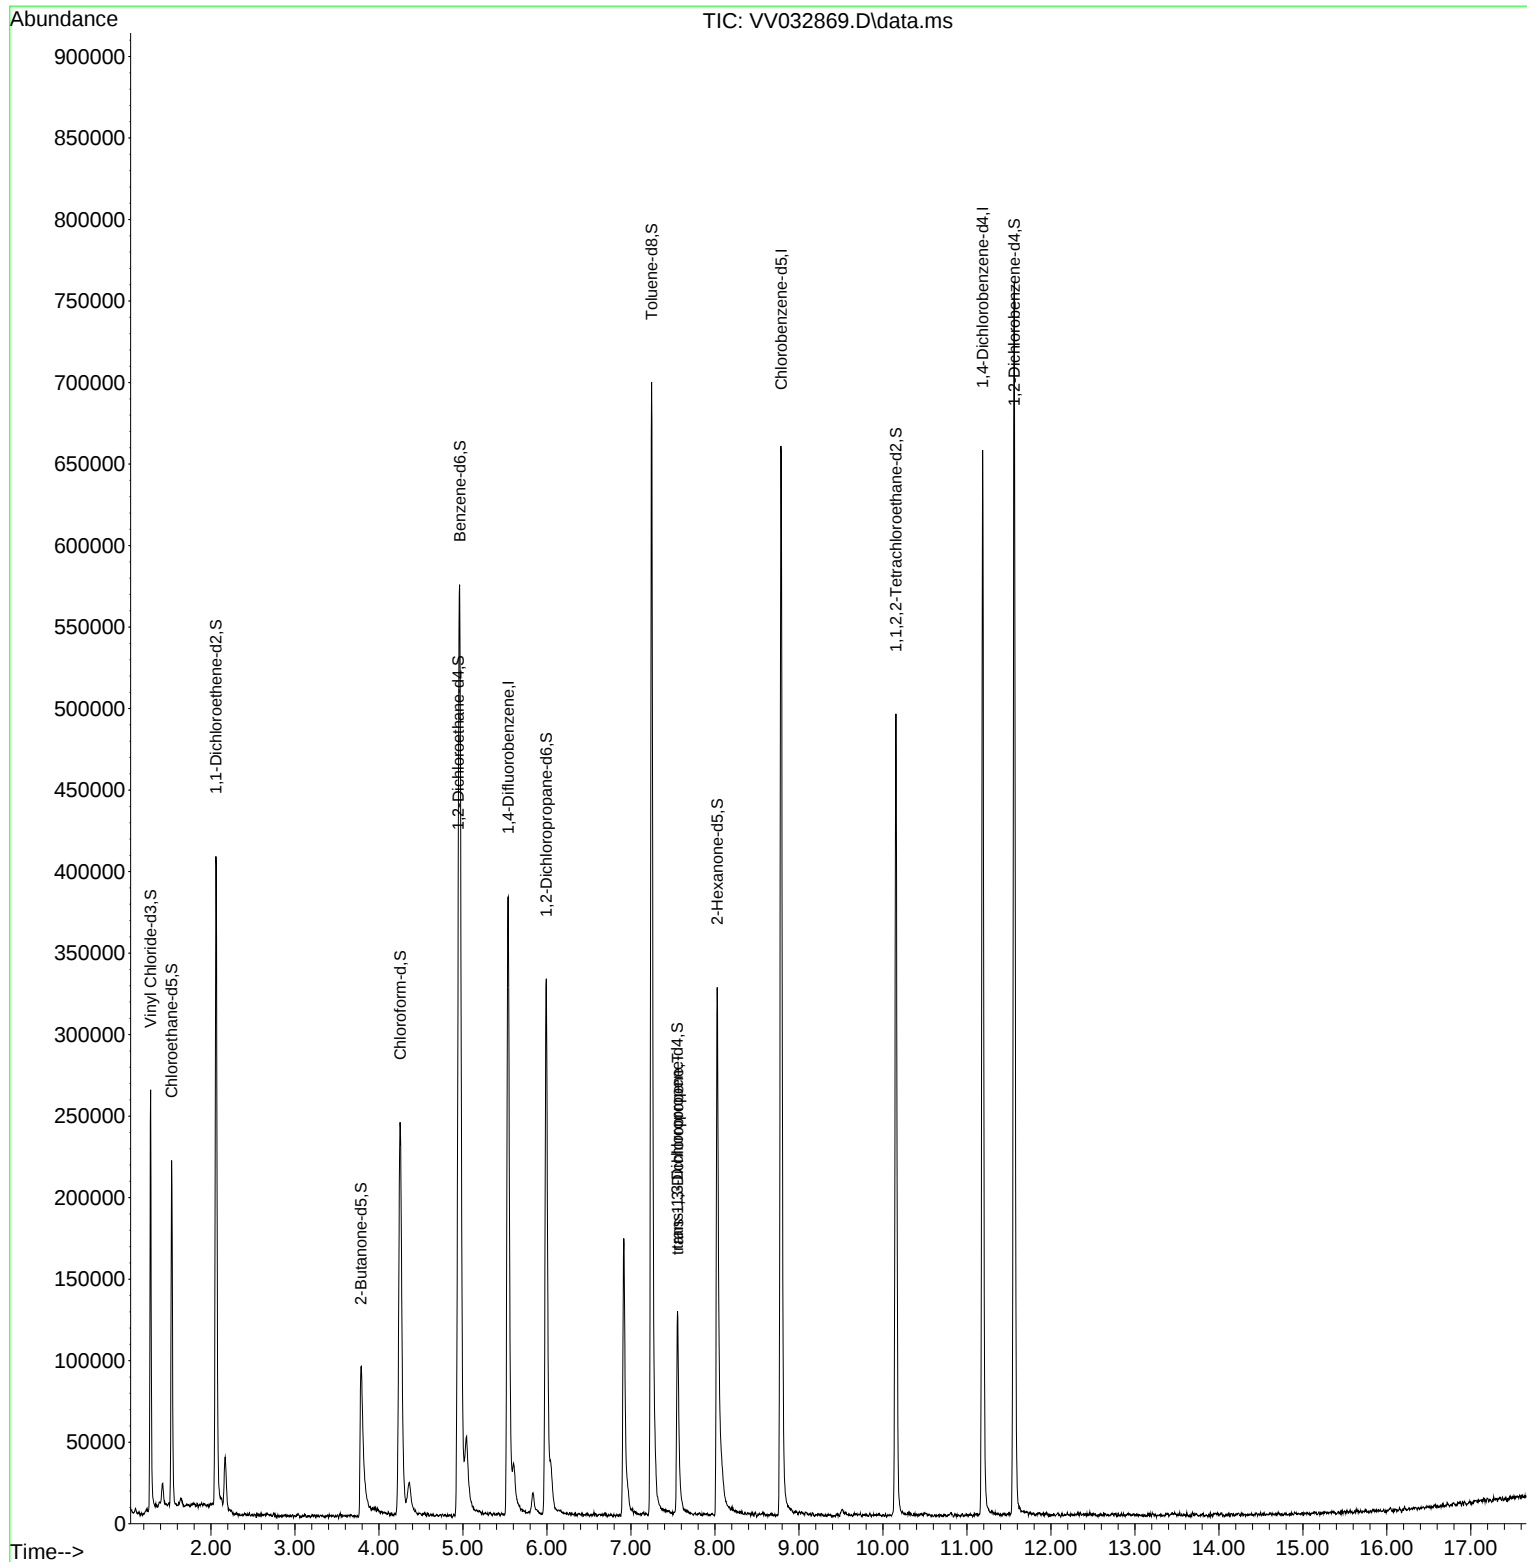

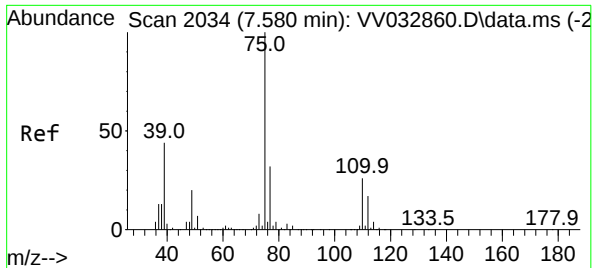

#44
 trans-1,3-Dichloropropene
 Concen: 1.012 ug/L
 RT: 7.558 min Scan# 20
 Delta R.T. -0.023 min
 Lab File: VV032869.D
 Acq: 07 Nov 2023 15:04

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4137
 Ion Ratio Lower Upper
 75 100
 77 54.9 22.0 40.8#

