

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110723\
 Data File : VW032865.D
 Acq On : 07 Nov 2023 13:31
 Operator : SY/MD
 Sample : 05226-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD2

Quant Time: Nov 08 01:38:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	318727	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	354147	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	158026	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	154709	51.034	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 102.060%		
7) Chloroethane-d5	1.532	69	131268	51.774	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 103.540%		
11) 1,1-Dichloroethene-d2	2.060	65	63987	51.102	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 102.200%		
21) 2-Butanone-d5	3.786	46	135733	103.225	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 103.220%		
24) Chloroform-d	4.249	84	248090	51.271	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 102.540%		
26) 1,2-Dichloroethane-d4	4.944	65	160712	53.439	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 106.880%		
32) Benzene-d6	4.963	84	493454	54.192	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 108.380%		
36) 1,2-Dichloropropane-d6	5.992	67	163380	59.060	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 118.120%		
41) Toluene-d8	7.246	98	469114	52.322	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 104.640%		
43) trans-1,3-Dichloroprop...	7.554	79	70565	48.978	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 97.960%		
47) 2-Hexanone-d5	8.027	63	98764	97.794	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 97.790%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	211403	50.359	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 100.720%		
66) 1,2-Dichlorobenzene-d4	11.564	152	183215	60.164	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	#120.320%		
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	18378	8.350	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032865.D
Acq On : 07 Nov 2023 13:31
Operator : SY/MD
Sample : 05226-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD2

Quant Time: Nov 08 01:38:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

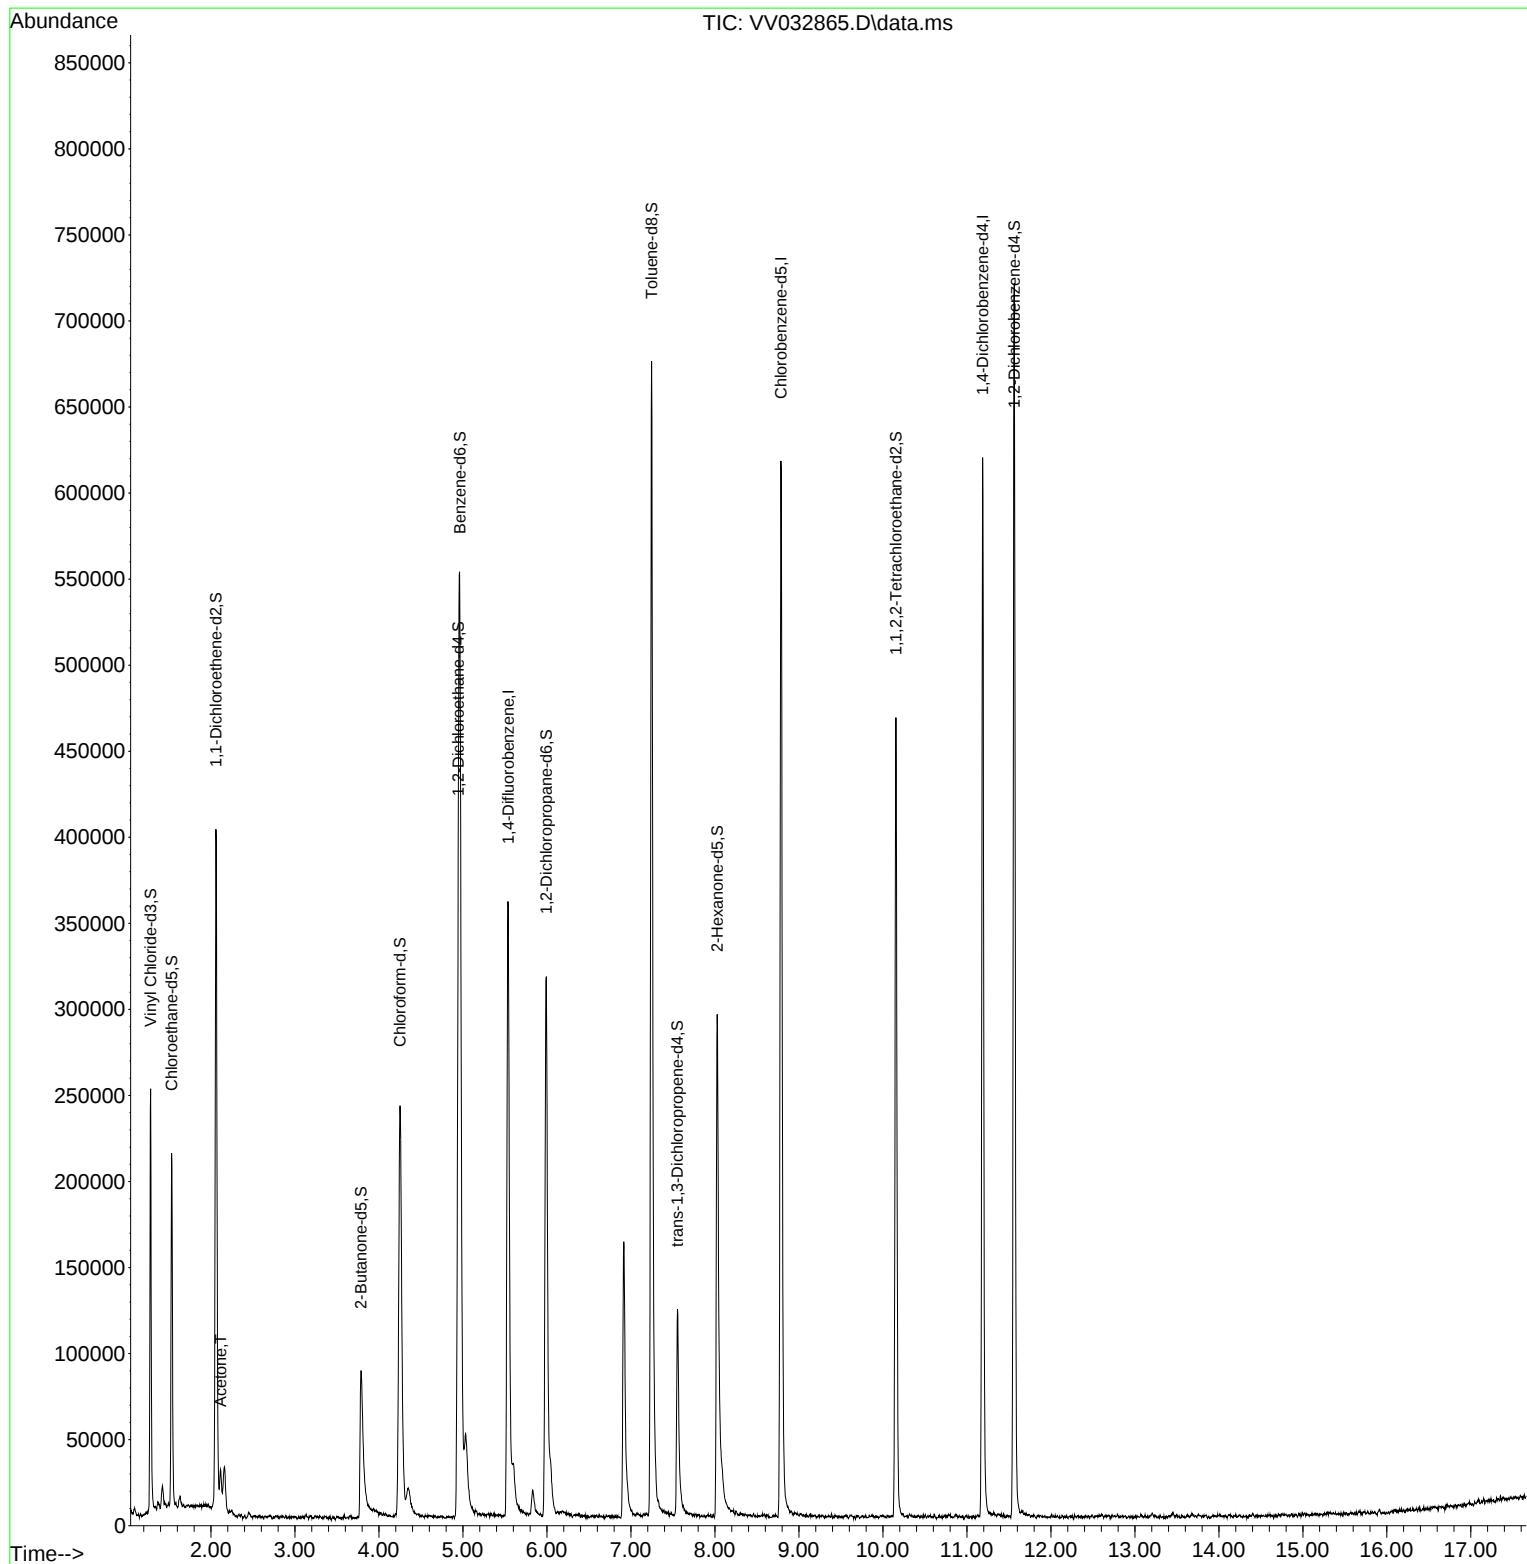

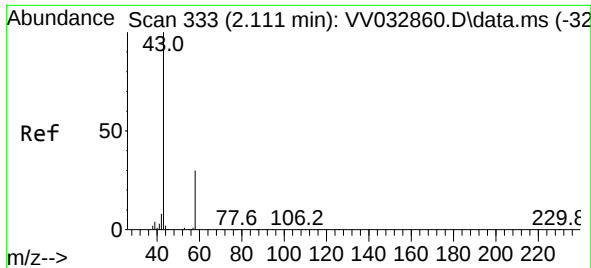

#13

Acetone

Concen: 8.350 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032865.D

Acq: 07 Nov 2023 13:31

Instrument :

MSVOA_V

ClientSampleId :

YCGD2

Tgt Ion: 43 Resp: 18378

Ion Ratio Lower Upper

43 100

58 35.4 0.0 61.2

