

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110723\
 Data File : VW032871.D
 Acq On : 07 Nov 2023 15:51
 Operator : SY/MD
 Sample : 05226-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD4

Quant Time: Nov 08 01:40:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	327342	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	362886	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	162659	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	152175	48.877	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	97.760%	
7) Chloroethane-d5	1.532	69	135473	52.026	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	104.060%	
11) 1,1-Dichloroethene-d2	2.063	65	65501	50.934	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	101.860%	
21) 2-Butanone-d5	3.786	46	146302	108.334	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	108.330%	
24) Chloroform-d	4.252	84	257417	51.798	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.600%	
26) 1,2-Dichloroethane-d4	4.944	65	164844	53.371	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.740%	
32) Benzene-d6	4.963	84	496769	53.242	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.480%	
36) 1,2-Dichloropropane-d6	5.992	67	150394	53.056	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	106.120%	
41) Toluene-d8	7.246	98	471693	51.342	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.680%	
43) trans-1,3-Dichloroprop...	7.554	79	71149	48.194	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.380%	
47) 2-Hexanone-d5	8.027	63	102894	99.430	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	99.430%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	221226	51.430	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	102.860%	
66) 1,2-Dichlorobenzene-d4	11.564	152	186910	59.629	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	119.260%	
Target Compounds						
13) Acetone	2.114	43	16579	7.334	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032871.D
Acq On : 07 Nov 2023 15:51
Operator : SY/MD
Sample : 05226-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD4

Quant Time: Nov 08 01:40:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

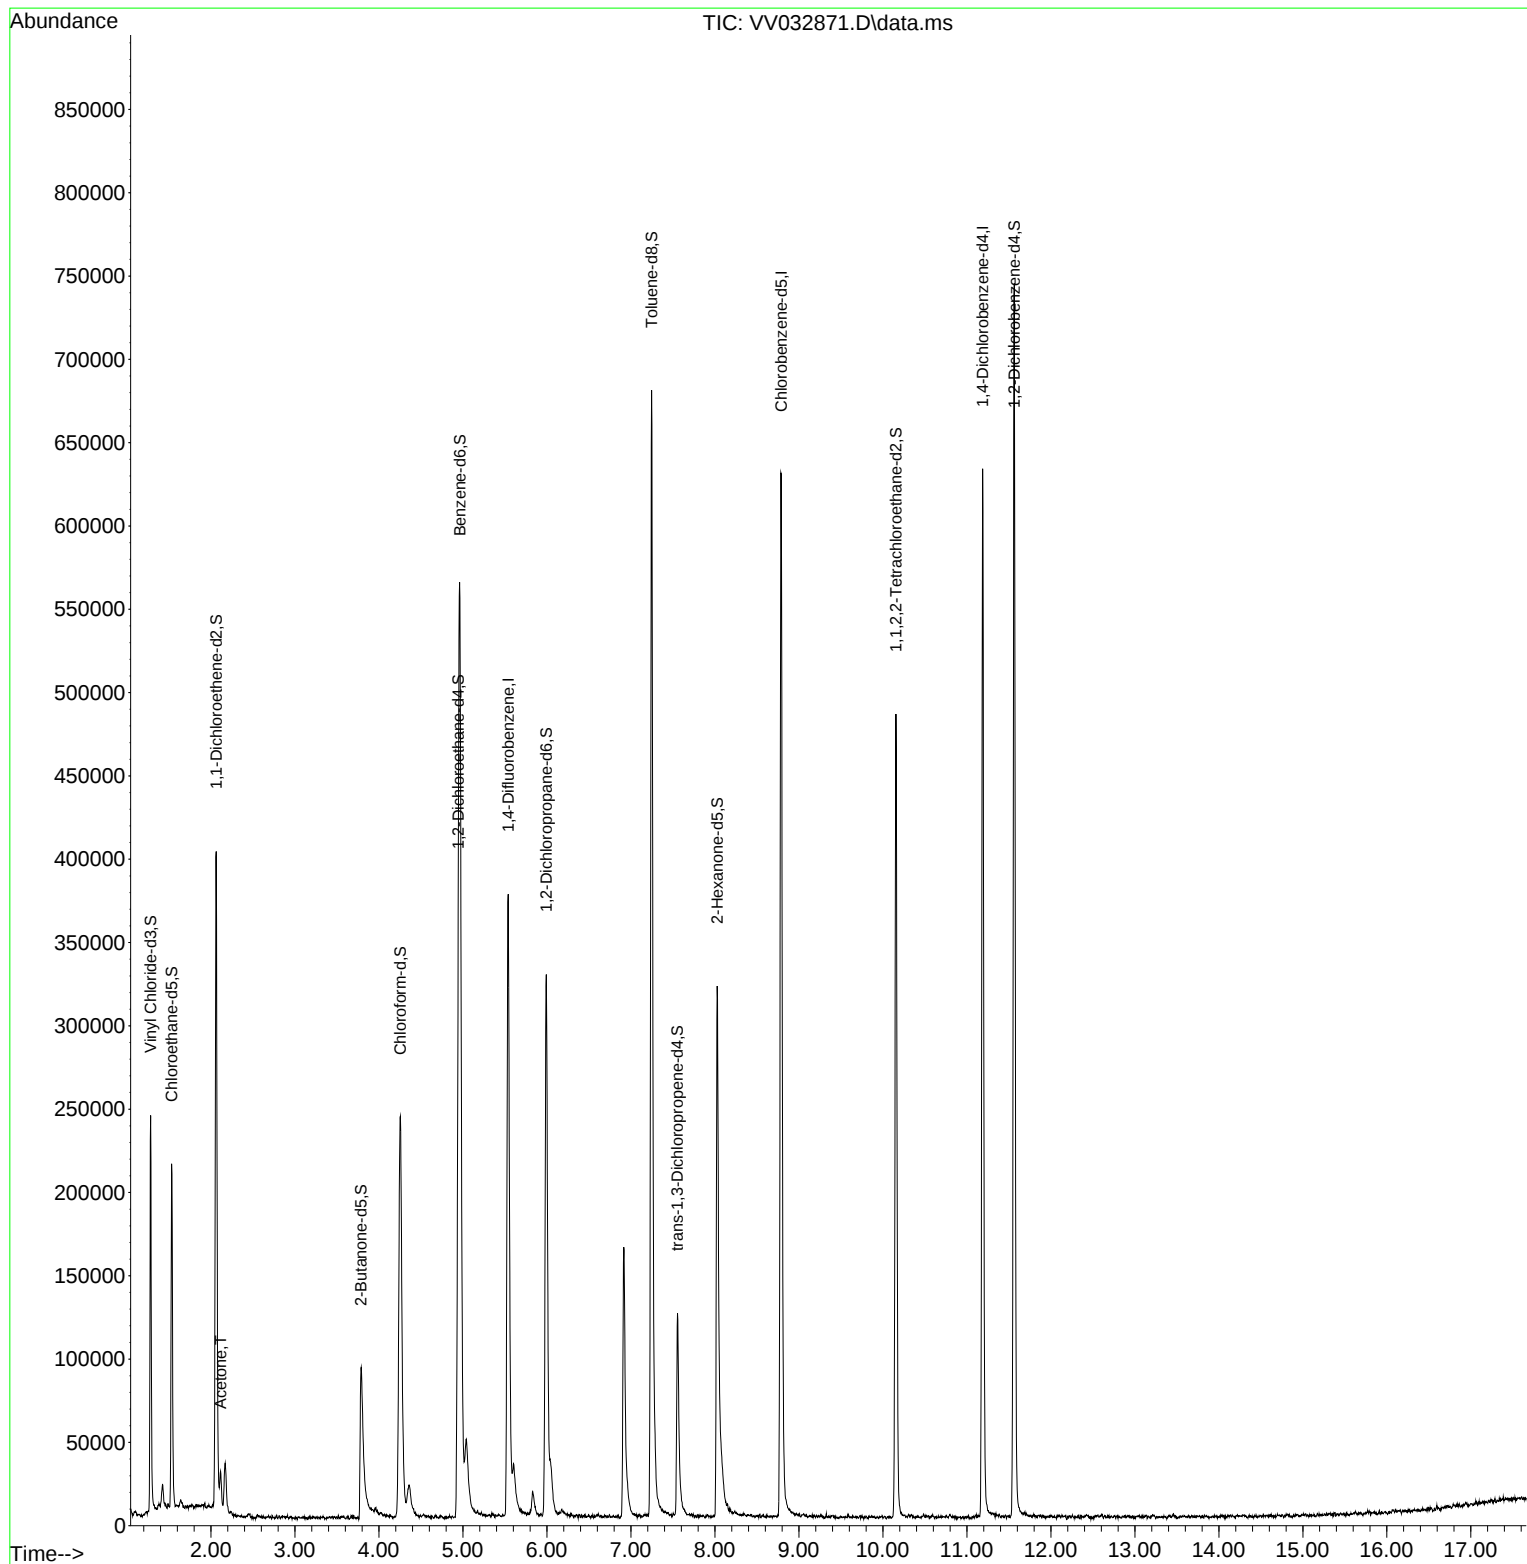

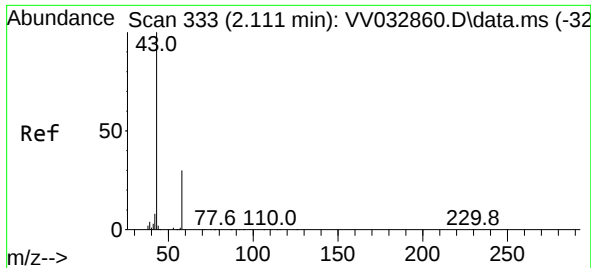

#13

Acetone

Concen: 7.334 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032871.D

Acq: 07 Nov 2023 15:51

Instrument :

MSVOA_V

ClientSampleId :

YCGD4

Tgt Ion: 43 Resp: 16579

Ion Ratio Lower Upper

43 100

58 38.0 0.0 61.2

