

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032862.D
 Acq On : 07 Nov 2023 12:03
 Operator : SY/MD
 Sample : VV1107WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rBV	229008	245558	16.50%	2.123%
2	1.532	147	153	165	rVB	199029	232285	15.61%	2.008%
3	2.059	308	317	331	rBV	382262	557956	37.49%	4.824%
4	2.378	414	416	426	rVB10	1942	2188	0.15%	0.019%
5	2.452	432	439	443	rBV7	4528	5333	0.36%	0.046%
6	2.587	479	481	484	rBV3	1768	896	0.06%	0.008%
7	2.613	487	489	491	rBV3	919	525	0.04%	0.005%
8	2.635	493	496	499	rBV5	1963	1262	0.08%	0.011%
9	2.664	503	505	506	rBV2	1525	581	0.04%	0.005%
10	2.793	543	545	547	rBV3	1237	526	0.04%	0.005%
11	2.834	555	558	560	rBV3	1622	1057	0.07%	0.009%
12	2.982	601	604	607	rBV6	1587	1242	0.08%	0.011%
13	3.011	610	613	616	rBV4	1397	941	0.06%	0.008%
14	3.066	628	630	631	rBV2	1268	426	0.03%	0.004%
15	3.095	636	639	642	rBV4	878	773	0.05%	0.007%
16	3.156	656	658	660	rBV2	955	304	0.02%	0.003%
17	3.220	676	678	679	rBV2	737	245	0.02%	0.002%
18	3.304	703	704	706	rVB3	933	199	0.01%	0.002%
19	3.317	706	708	712	rBV5	1235	965	0.06%	0.008%
20	3.336	712	714	716	rBV3	1002	521	0.04%	0.005%
21	3.410	735	737	742	rVB5	1589	1271	0.09%	0.011%
22	3.432	742	744	745	rBV2	1726	632	0.04%	0.005%
23	3.616	797	801	803	rBV5	1543	1194	0.08%	0.010%
24	3.654	811	813	815	rBV3	1255	503	0.03%	0.004%
25	3.731	835	837	839	rBV3	1073	539	0.04%	0.005%
26	3.748	839	842	843	rBV3	1012	449	0.03%	0.004%
27	3.783	844	853	883	rBV	87394	248452	16.69%	2.148%
28	4.249	985	998	1017	rBV	233666	587003	39.44%	5.075%
29	4.715	1139	1143	1144	rBV4	1458	755	0.05%	0.007%
30	4.802	1167	1170	1173	rBV5	1558	957	0.06%	0.008%
31	4.821	1174	1176	1179	rBV4	1764	1107	0.07%	0.010%
32	4.886	1194	1196	1197	rBV2	929	309	0.02%	0.003%
33	4.956	1201	1218	1235	rBV2	560632	1488232	100.00%	12.867%
34	5.493	1383	1385	1386	rBV2	1391	657	0.04%	0.006%
35	5.532	1386	1397	1412	rBV	384947	793808	53.34%	6.863%
36	5.989	1527	1539	1573	rBV	324974	728292	48.94%	6.297%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032862.D
 Acq On : 07 Nov 2023 12:03
 Operator : SY/MD
 Sample : VV1107WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.255	1620	1622	1626	rVB4	1700	1135	0.08%	0.010%
38	6.413	1668	1671	1673	rBV4	1404	830	0.06%	0.007%
39	6.436	1676	1678	1680	rBV2	1454	879	0.06%	0.008%
40	6.458	1683	1685	1687	rBV3	1300	737	0.05%	0.006%
41	6.554	1713	1715	1717	rBV3	979	475	0.03%	0.004%
42	6.796	1788	1790	1791	rBV2	1051	449	0.03%	0.004%
43	6.915	1817	1827	1860	rBV	167290	348488	23.42%	3.013%
44	7.243	1918	1929	1963	rBV	681257	1272719	85.52%	11.004%
45	7.551	2017	2025	2045	rBV	123436	229667	15.43%	1.986%
46	7.760	2087	2090	2091	rBV3	1828	1042	0.07%	0.009%
47	8.027	2163	2173	2203	rBV	286139	617139	41.47%	5.336%
48	8.468	2305	2310	2314	rBV7	1262	1490	0.10%	0.013%
49	8.503	2318	2321	2325	rVB5	1635	1163	0.08%	0.010%
50	8.587	2342	2347	2351	rVB7	1831	1779	0.12%	0.015%
51	8.786	2398	2409	2430	rBV	667314	1133846	76.19%	9.803%
52	9.098	2504	2506	2507	rBV2	1545	502	0.03%	0.004%
53	9.210	2539	2541	2544	rBV4	2341	1393	0.09%	0.012%
54	9.336	2578	2580	2581	rBV2	1329	438	0.03%	0.004%
55	9.513	2633	2635	2638	rBV4	1427	882	0.06%	0.008%
56	9.664	2680	2682	2685	rBV4	1435	742	0.05%	0.006%
57	9.705	2694	2695	2698	rVB3	1467	538	0.04%	0.005%
58	9.725	2698	2701	2705	rBV5	1951	1336	0.09%	0.012%
59	9.754	2708	2710	2712	rBV2	1001	553	0.04%	0.005%
60	10.001	2786	2787	2788	rBV	1147	382	0.03%	0.003%
61	10.152	2823	2834	2852	rBV	483530	761805	51.19%	6.587%
62	10.365	2898	2900	2902	rBV3	1051	465	0.03%	0.004%
63	10.442	2920	2924	2929	rBV8	1860	1905	0.13%	0.016%
64	10.522	2946	2949	2950	rBV3	1416	736	0.05%	0.006%
65	10.673	2993	2996	2998	rBV4	1415	894	0.06%	0.008%
66	10.902	3061	3067	3070	rBV8	2190	2053	0.14%	0.018%
67	10.947	3078	3081	3083	rBV4	1669	1086	0.07%	0.009%
68	11.001	3096	3098	3101	rBV2	1646	747	0.05%	0.006%
69	11.188	3145	3156	3181	rBV	665074	1054698	70.87%	9.119%
70	11.561	3261	3272	3289	rBV	746302	1190650	80.00%	10.295%
71	11.773	3336	3338	3340	rBV3	1883	919	0.06%	0.008%
72	11.834	3354	3357	3360	rBV5	1260	977	0.07%	0.008%
73	11.918	3380	3383	3385	rBV4	1377	1036	0.07%	0.009%
74	12.271	3491	3493	3494	rBV2	1776	615	0.04%	0.005%
75	12.416	3536	3538	3540	rBV3	1575	672	0.05%	0.006%
76	12.590	3585	3592	3597	rBV10	2627	4361	0.29%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032862.D
 Acq On : 07 Nov 2023 12:03
 Operator : SY/MD
 Sample : VV1107WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	12.747	3639	3641	3643	rBV3	1868	1006	0.07%	0.009%
78	12.847	3670	3672	3675	rBV4	1606	925	0.06%	0.008%
79	12.966	3708	3709	3716	rVB6	2089	1727	0.12%	0.015%
80	12.998	3716	3719	3722	rBV4	2008	1628	0.11%	0.014%
81	13.117	3754	3756	3758	rBV3	1100	401	0.03%	0.003%
82	13.155	3766	3768	3770	rVB2	1384	440	0.03%	0.004%
83	13.168	3770	3772	3773	rBV3	1115	372	0.02%	0.003%
84	13.326	3819	3821	3822	rBV2	1402	527	0.04%	0.005%
85	13.988	4024	4027	4028	rBV2	1384	627	0.04%	0.005%
86	14.033	4039	4041	4044	rVB4	2494	1098	0.07%	0.009%
87	14.049	4044	4046	4048	rBV3	1830	919	0.06%	0.008%
88	14.342	4133	4137	4140	rBV4	2017	1784	0.12%	0.015%
89	14.358	4140	4142	4144	rVB3	1818	685	0.05%	0.006%
90	14.461	4170	4174	4177	rBV5	2016	1943	0.13%	0.017%
91	14.506	4186	4188	4192	rBV6	2312	1613	0.11%	0.014%




Sum of corrected areas: 11565861

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032862.D
Acq On : 07 Nov 2023 12:03
Operator : SY/MD
Sample : VV1107WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

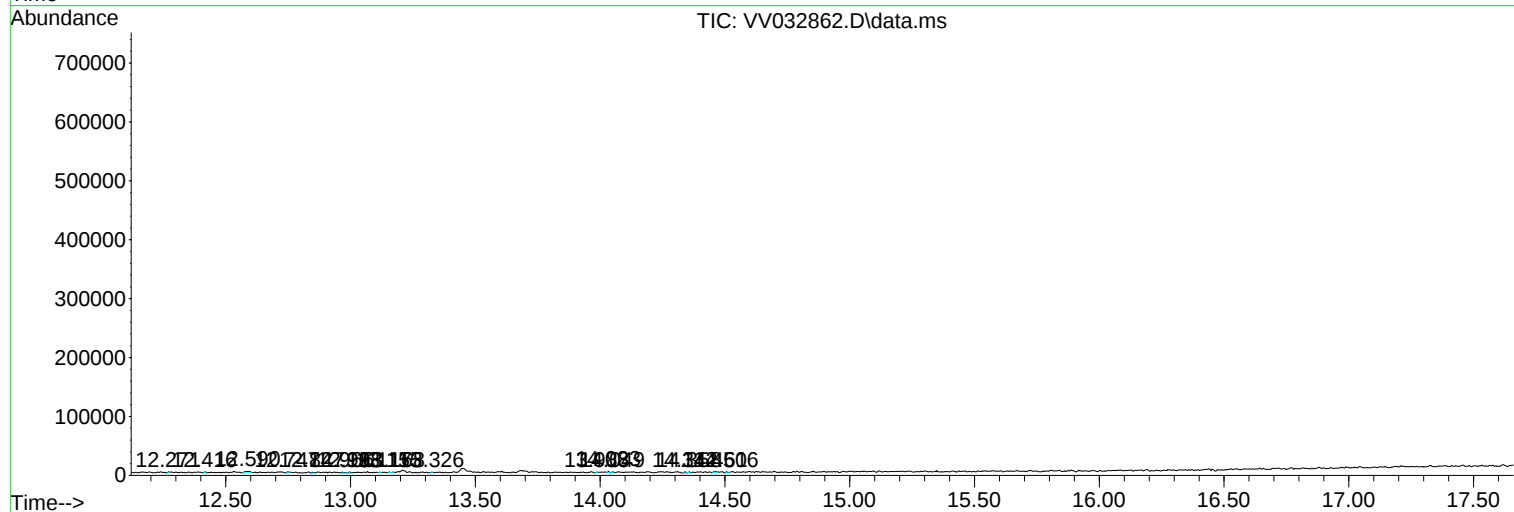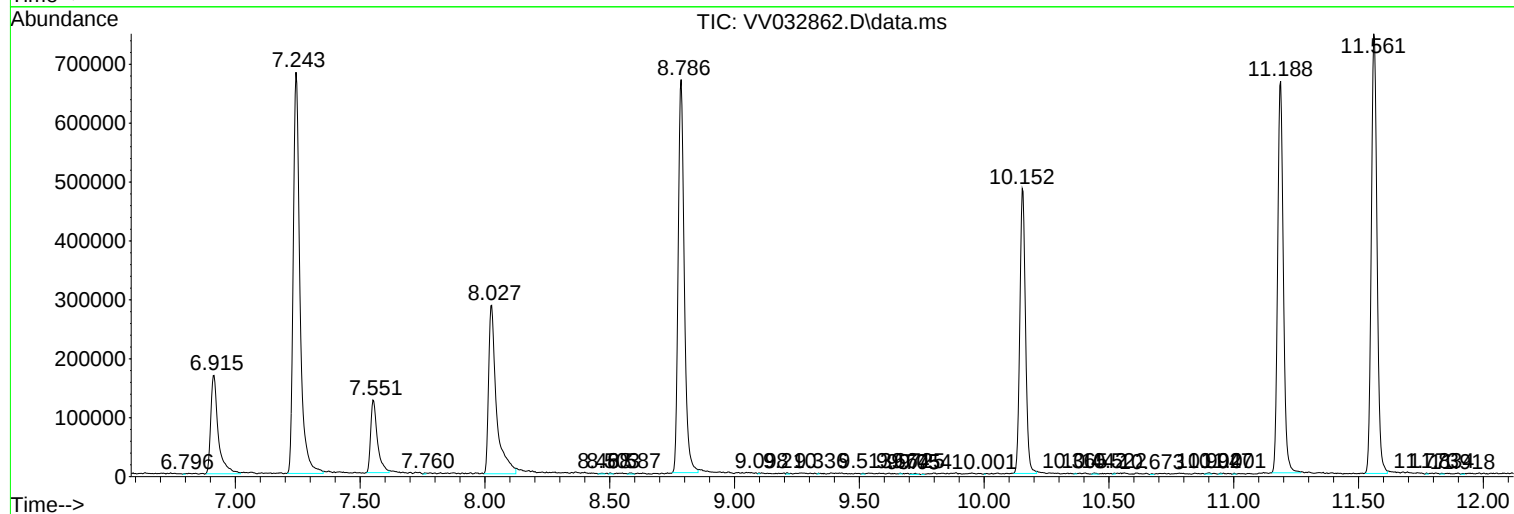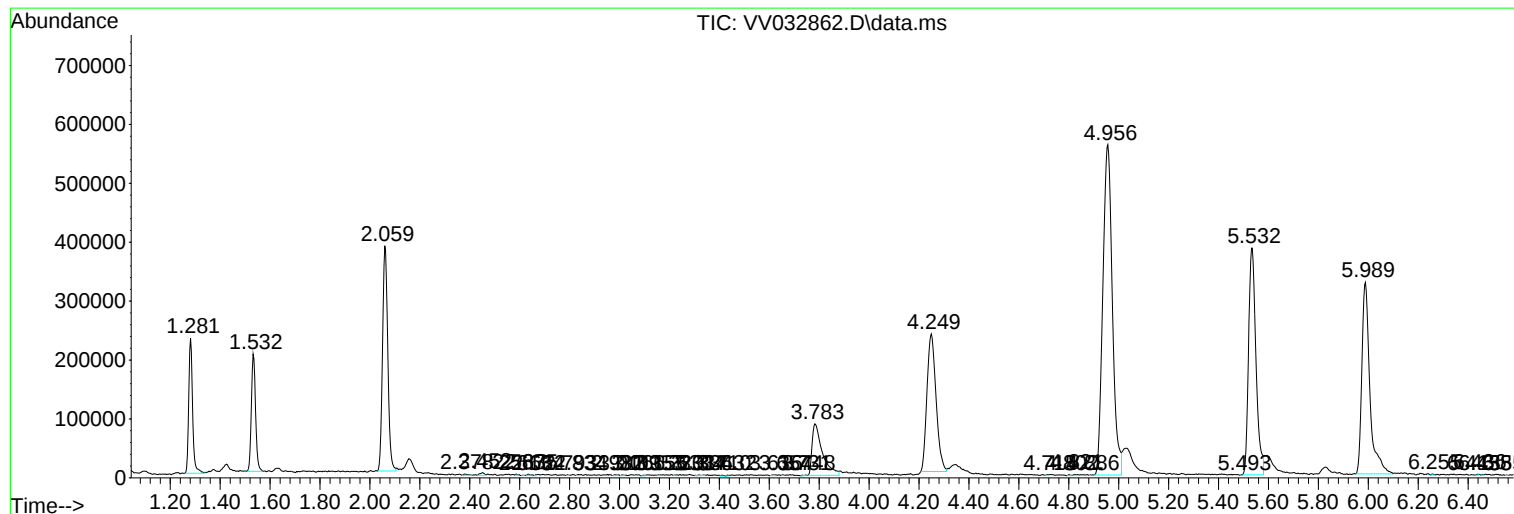

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032862.D
Acq On : 07 Nov 2023 12:03
Operator : SY/MD
Sample : VV1107WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032862.D
Acq On : 07 Nov 2023 12:03
Operator : SY/MD
Sample : VV1107WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc