

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032865.D
 Acq On : 07 Nov 2023 13:31
 Operator : SY/MD
 Sample : 05226-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rBV	243791	251420	17.41%	2.259%
2	1.532	146	153	165	rVB	204477	237913	16.47%	2.138%
3	2.060	309	317	329	rBV	386993	550813	38.14%	4.949%
4	2.381	415	417	419	rBV3	1051	539	0.04%	0.005%
5	2.638	493	497	499	rBV5	1758	1420	0.10%	0.013%
6	2.744	526	530	533	rBV6	1340	958	0.07%	0.009%
7	2.773	533	539	541	rBV5	1494	1444	0.10%	0.013%
8	2.825	551	555	558	rBV6	1713	1854	0.13%	0.017%
9	2.918	580	584	586	rBV5	1277	992	0.07%	0.009%
10	2.931	586	588	590	rVB3	1562	579	0.04%	0.005%
11	3.043	621	623	626	rVB3	1251	523	0.04%	0.005%
12	3.059	626	628	630	rBV3	981	447	0.03%	0.004%
13	3.169	660	662	664	rBV3	1834	1061	0.07%	0.010%
14	3.236	680	683	686	rBV5	1498	1242	0.09%	0.011%
15	3.291	698	700	702	rBV3	1504	786	0.05%	0.007%
16	3.330	710	712	714	rBV3	1150	543	0.04%	0.005%
17	3.349	716	718	721	rBV4	1439	995	0.07%	0.009%
18	3.416	734	739	741	rBV5	1904	1402	0.10%	0.013%
19	3.452	744	750	753	rBV6	2155	2168	0.15%	0.019%
20	3.465	753	754	759	rVB5	1761	1026	0.07%	0.009%
21	3.497	762	764	766	rBV3	939	382	0.03%	0.003%
22	3.564	783	785	787	rBV3	1335	805	0.06%	0.007%
23	3.587	789	792	797	rVV7	2571	1880	0.13%	0.017%
24	3.651	809	812	815	rBV5	1423	1237	0.09%	0.011%
25	3.690	821	824	826	rBV5	1134	776	0.05%	0.007%
26	3.786	845	854	882	rBV	85525	239095	16.55%	2.148%
27	4.252	986	999	1019	rBV2	234717	589096	40.79%	5.293%
28	4.699	1136	1138	1139	rBV2	934	283	0.02%	0.003%
29	4.960	1203	1219	1235	rBV2	548458	1444247	100.00%	12.977%
30	5.535	1387	1398	1413	rBV	357198	734425	50.85%	6.599%
31	5.992	1528	1540	1576	rBV	312388	710451	49.19%	6.384%
32	6.458	1684	1685	1687	rVB2	1979	525	0.04%	0.005%
33	6.481	1687	1692	1694	rBV6	2058	1697	0.12%	0.015%
34	6.493	1694	1696	1700	rBV5	1234	778	0.05%	0.007%
35	6.693	1756	1758	1760	rBV3	1066	653	0.05%	0.006%
36	6.706	1760	1762	1767	rVV6	1690	1452	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032865.D
 Acq On : 07 Nov 2023 13:31
 Operator : SY/MD
 Sample : 05226-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.764	1778	1780	1782	rBV3	1191	486	0.03%	0.004%
38	6.776	1782	1784	1787	rVB4	1626	956	0.07%	0.009%
39	6.792	1787	1789	1792	rBV4	1188	727	0.05%	0.007%
40	6.844	1802	1805	1808	rBV5	1583	918	0.06%	0.008%
41	6.915	1817	1827	1855	rBV	159905	333107	23.06%	2.993%
42	7.246	1919	1930	1962	rBV	670061	1241235	85.94%	11.153%
43	7.554	2018	2026	2045	rBV	117763	214646	14.86%	1.929%
44	8.027	2163	2173	2205	rBV2	292395	634853	43.96%	5.704%
45	8.786	2398	2409	2434	rBV	613811	1053016	72.91%	9.462%
46	9.091	2502	2504	2507	rBV3	1515	739	0.05%	0.007%
47	9.217	2540	2543	2545	rBV4	1253	823	0.06%	0.007%
48	9.316	2570	2574	2576	rBV6	1640	1144	0.08%	0.010%
49	9.429	2607	2609	2612	rBV4	1773	1056	0.07%	0.009%
50	9.468	2618	2621	2623	rBV4	1341	766	0.05%	0.007%
51	9.532	2639	2641	2642	rBV2	1120	455	0.03%	0.004%
52	9.657	2678	2680	2681	rBV2	1303	586	0.04%	0.005%
53	9.683	2685	2688	2691	rBV5	2340	1808	0.13%	0.016%
54	10.156	2824	2835	2856	rBV	464416	736682	51.01%	6.619%
55	10.316	2880	2885	2889	rBV8	2333	2698	0.19%	0.024%
56	10.458	2927	2929	2931	rBV3	1084	520	0.04%	0.005%
57	10.480	2934	2936	2938	rBV3	1890	741	0.05%	0.007%
58	10.609	2974	2976	2985	rVB8	2966	2970	0.21%	0.027%
59	10.641	2985	2986	2990	rBV4	1141	872	0.06%	0.008%
60	10.696	3002	3003	3005	rBV2	995	315	0.02%	0.003%
61	10.783	3025	3030	3032	rBV5	1937	1664	0.12%	0.015%
62	11.033	3106	3108	3109	rBV3	1206	560	0.04%	0.005%
63	11.069	3116	3119	3120	rBV3	1470	857	0.06%	0.008%
64	11.104	3128	3130	3132	rBV3	1523	761	0.05%	0.007%
65	11.188	3145	3156	3178	rBV	615459	947421	65.60%	8.513%
66	11.410	3223	3225	3228	rVB4	1853	870	0.06%	0.008%
67	11.564	3261	3273	3295	rBV	716095	1141931	79.07%	10.260%
68	11.840	3355	3359	3360	rBV4	1680	1290	0.09%	0.012%
69	12.217	3472	3476	3477	rBV4	1180	1033	0.07%	0.009%
70	12.281	3493	3496	3498	rBV4	2832	1644	0.11%	0.015%
71	12.381	3525	3527	3529	rBV3	1203	622	0.04%	0.006%
72	12.638	3604	3607	3609	rBV4	1344	870	0.06%	0.008%
73	12.721	3628	3633	3634	rBV5	1842	1517	0.11%	0.014%
74	12.731	3634	3636	3641	rVV5	1682	1504	0.10%	0.014%
75	13.011	3720	3723	3725	rVB4	1781	929	0.06%	0.008%
76	13.152	3765	3767	3769	rVB3	1580	628	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032865.D
Acq On : 07 Nov 2023 13:31
Operator : SY/MD
Sample : 05226-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	13.300	3810	3813	3818	rBV5	2100	1609	0.11%	0.014%
78	13.345	3826	3827	3832	rVB5	1732	739	0.05%	0.007%
79	13.368	3832	3834	3836	rBV3	1696	971	0.07%	0.009%
80	13.744	3949	3951	3952	rBV2	1331	594	0.04%	0.005%
81	13.895	3996	3998	4000	rVB3	1105	490	0.03%	0.004%
82	14.178	4083	4086	4089	rBV4	1617	1199	0.08%	0.011%
83	14.361	4140	4143	4146	rBV5	1829	1673	0.12%	0.015%




Sum of corrected areas: 11129402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032865.D
Acq On : 07 Nov 2023 13:31
Operator : SY/MD
Sample : 05226-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

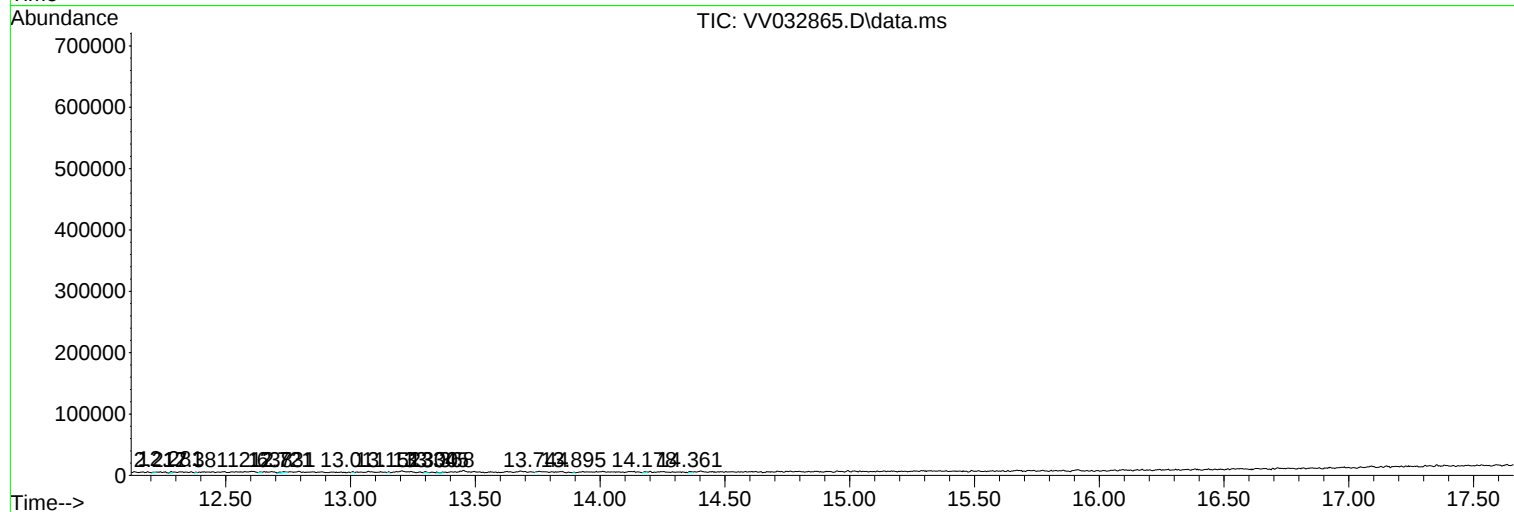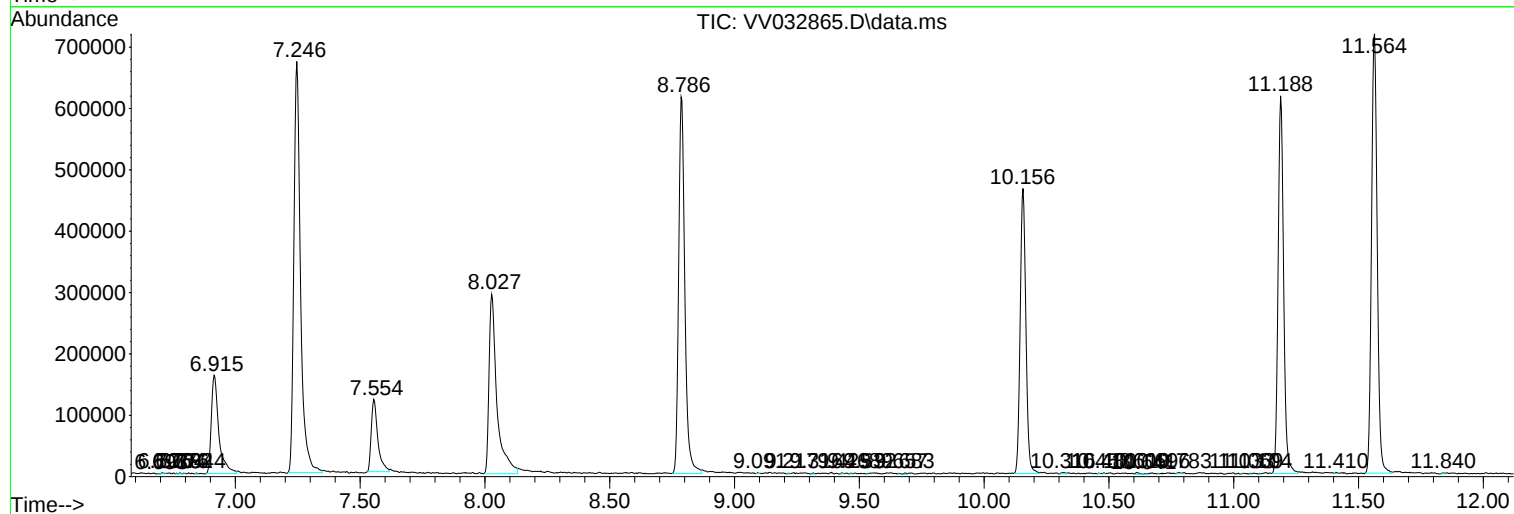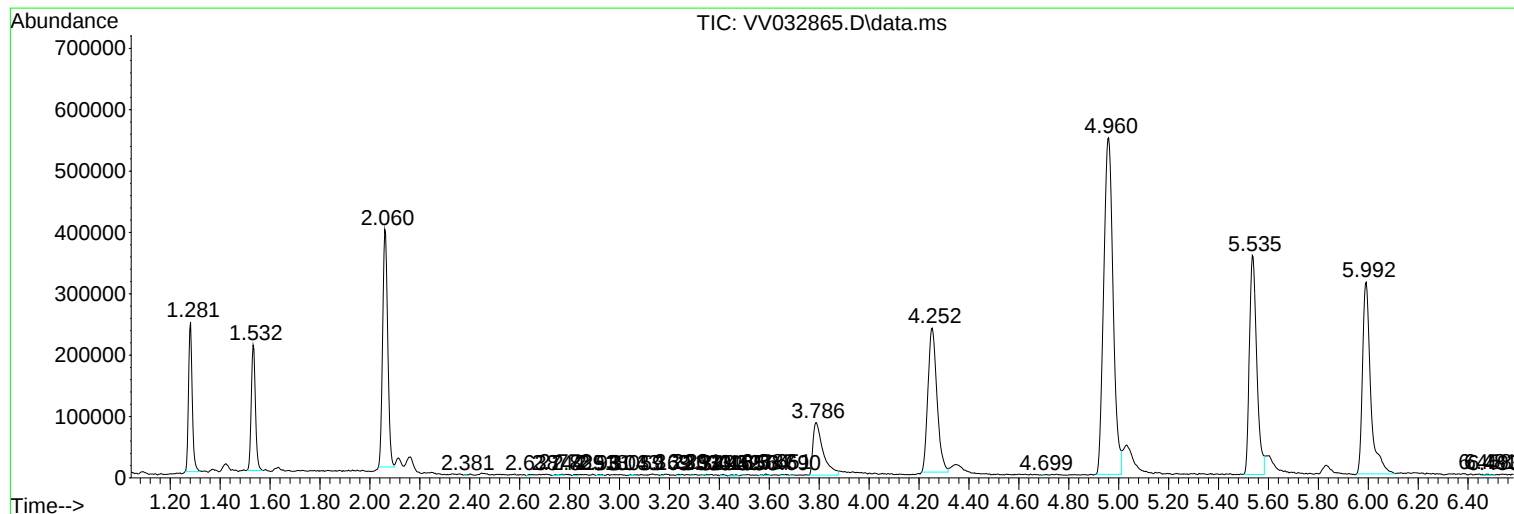

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032865.D
Acq On : 07 Nov 2023 13:31
Operator : SY/MD
Sample : 05226-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032865.D
Acq On : 07 Nov 2023 13:31
Operator : SY/MD
Sample : 05226-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc