

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032866.D
 Acq On : 07 Nov 2023 13:54
 Operator : SY/MD
 Sample : 05226-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.153	33	35	39	rBV6	2099	1859	0.12%	0.016%
2	1.282	68	75	91	rVB	248885	268128	17.68%	2.280%
3	1.532	146	153	167	rVB	212384	251199	16.56%	2.136%
4	2.060	309	317	335	rVB	402784	581662	38.34%	4.947%
5	2.323	397	399	402	rBV4	1964	1073	0.07%	0.009%
6	2.581	477	479	483	rBV5	1854	1247	0.08%	0.011%
7	2.661	502	504	507	rBV3	1101	719	0.05%	0.006%
8	2.761	533	535	537	rBV2	1159	610	0.04%	0.005%
9	2.793	543	545	547	rBV3	914	552	0.04%	0.005%
10	2.835	554	558	559	rBV3	972	616	0.04%	0.005%
11	2.870	566	569	570	rBV4	1089	457	0.03%	0.004%
12	2.937	586	590	591	rBV3	1824	1513	0.10%	0.013%
13	3.272	690	694	698	rVB7	1820	1312	0.09%	0.011%
14	3.291	698	700	702	rBV3	1113	535	0.04%	0.005%
15	3.336	712	714	718	rBV5	1620	847	0.06%	0.007%
16	3.394	730	732	735	rBV4	925	629	0.04%	0.005%
17	3.452	748	750	755	rVB6	1590	1066	0.07%	0.009%
18	3.487	755	761	762	rBV5	1074	781	0.05%	0.007%
19	3.536	774	776	779	rVB4	503	223	0.01%	0.002%
20	3.558	779	783	785	rBV5	1642	1304	0.09%	0.011%
21	3.590	791	793	795	rBV3	1018	484	0.03%	0.004%
22	3.603	795	797	798	rBV2	788	313	0.02%	0.003%
23	3.635	802	807	809	rBV6	1980	2015	0.13%	0.017%
24	3.719	831	833	834	rBV2	1023	276	0.02%	0.002%
25	3.738	837	839	841	rBV3	862	397	0.03%	0.003%
26	3.754	841	844	846	rBV4	1413	983	0.06%	0.008%
27	3.786	846	854	877	rBV2	86518	228801	15.08%	1.946%
28	4.253	984	999	1019	rBV2	248399	637264	42.01%	5.420%
29	4.687	1132	1134	1137	rVB5	1939	744	0.05%	0.006%
30	4.716	1137	1143	1145	rBV5	2106	1881	0.12%	0.016%
31	4.754	1153	1155	1156	rBV2	653	314	0.02%	0.003%
32	4.764	1156	1158	1163	rVV6	2169	2229	0.15%	0.019%
33	4.786	1163	1165	1168	rVV4	2104	1363	0.09%	0.012%
34	4.809	1170	1172	1173	rVB2	1274	389	0.03%	0.003%
35	4.818	1173	1175	1178	rBV5	1283	747	0.05%	0.006%
36	4.851	1183	1185	1186	rBV2	1020	394	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032866.D
 Acq On : 07 Nov 2023 13:54
 Operator : SY/MD
 Sample : 05226-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.876	1191	1193	1199	rVB7	1587	1364	0.09%	0.012%
38	4.905	1200	1202	1203	rBV	1523	546	0.04%	0.005%
39	4.960	1203	1219	1235	rBV2	576629	1516923	100.00%	12.901%
40	5.433	1364	1366	1368	rBV3	983	699	0.05%	0.006%
41	5.535	1387	1398	1413	rBV	382854	782559	51.59%	6.656%
42	5.921	1515	1518	1523	rBV6	1719	1486	0.10%	0.013%
43	5.992	1528	1540	1570	rVV	327060	734970	48.45%	6.251%
44	6.362	1649	1655	1659	rBV7	2693	3501	0.23%	0.030%
45	6.664	1747	1749	1751	rBV3	1432	688	0.05%	0.006%
46	6.764	1777	1780	1786	rBV7	2527	2332	0.15%	0.020%
47	6.796	1788	1790	1791	rBV2	1194	273	0.02%	0.002%
48	6.838	1800	1803	1805	rBV3	2441	1452	0.10%	0.012%
49	6.915	1814	1827	1854	rBV	172258	360300	23.75%	3.064%
50	7.137	1894	1896	1897	rBV2	1149	368	0.02%	0.003%
51	7.246	1919	1930	1959	rBV	708363	1315090	86.69%	11.185%
52	7.555	2018	2026	2046	rBV	120537	228539	15.07%	1.944%
53	7.969	2150	2155	2158	rBV7	1915	2142	0.14%	0.018%
54	8.027	2164	2173	2202	rBV	313167	648858	42.77%	5.519%
55	8.622	2354	2358	2361	rBV6	1949	1765	0.12%	0.015%
56	8.786	2399	2409	2432	rBV	660903	1098730	72.43%	9.345%
57	9.175	2527	2530	2532	rVB4	1802	785	0.05%	0.007%
58	9.194	2534	2536	2539	rBV4	1776	1010	0.07%	0.009%
59	9.243	2545	2551	2554	rBV7	2739	3079	0.20%	0.026%
60	9.612	2663	2666	2669	rBV5	1509	1131	0.07%	0.010%
61	9.738	2702	2705	2709	rBV6	1586	1724	0.11%	0.015%
62	9.757	2709	2711	2714	rVV4	1194	514	0.03%	0.004%
63	9.789	2719	2721	2723	rBV3	1466	756	0.05%	0.006%
64	9.911	2756	2759	2765	rVB7	1871	1925	0.13%	0.016%
65	9.947	2765	2770	2771	rBV5	1418	1113	0.07%	0.009%
66	10.027	2793	2795	2796	rBV2	1295	498	0.03%	0.004%
67	10.156	2824	2835	2851	rBV	505947	795807	52.46%	6.768%
68	10.532	2949	2952	2955	rBV3	1518	940	0.06%	0.008%
69	10.545	2955	2956	2959	rBV3	695	346	0.02%	0.003%
70	10.561	2959	2961	2962	rBV2	1227	506	0.03%	0.004%
71	10.847	3048	3050	3053	rVB4	1835	803	0.05%	0.007%
72	10.866	3053	3056	3058	rBV4	1687	957	0.06%	0.008%
73	10.921	3071	3073	3074	rBV2	966	514	0.03%	0.004%
74	10.979	3089	3091	3092	rBV2	1010	377	0.02%	0.003%
75	11.021	3100	3104	3105	rBV4	1643	1202	0.08%	0.010%
76	11.063	3116	3117	3118	rBV	1057	369	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032866.D
 Acq On : 07 Nov 2023 13:54
 Operator : SY/MD
 Sample : 05226-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.188	3145	3156	3178	rBV	648742	1006414	66.35%	8.560%
78	11.516	3254	3258	3260	rBV6	1671	1256	0.08%	0.011%
79	11.564	3261	3273	3291	rVV	771224	1218420	80.32%	10.363%
80	11.799	3344	3346	3349	rBV4	1870	1047	0.07%	0.009%
81	12.104	3439	3441	3443	rBV3	1498	742	0.05%	0.006%
82	12.284	3494	3497	3498	rBV3	830	427	0.03%	0.004%
83	12.326	3507	3510	3511	rBV3	1474	730	0.05%	0.006%
84	12.452	3547	3549	3550	rBV2	973	373	0.02%	0.003%
85	12.461	3550	3552	3553	rBV2	1429	731	0.05%	0.006%
86	12.590	3588	3592	3594	rBV5	1790	1581	0.10%	0.013%
87	12.673	3615	3618	3620	rBV4	1327	948	0.06%	0.008%
88	12.815	3660	3662	3665	rVB4	1371	551	0.04%	0.005%
89	12.873	3678	3680	3681	rBV2	1518	474	0.03%	0.004%
90	12.924	3693	3696	3698	rBV3	1989	1212	0.08%	0.010%
91	13.169	3770	3772	3774	rBV3	1559	641	0.04%	0.005%
92	13.185	3774	3777	3779	rBV4	1376	951	0.06%	0.008%
93	13.442	3852	3857	3859	rBV5	2355	1961	0.13%	0.017%
94	13.632	3912	3916	3917	rBV3	2508	1646	0.11%	0.014%
95	13.657	3922	3924	3925	rBV2	1218	394	0.03%	0.003%
96	13.712	3939	3941	3942	rBV2	1239	458	0.03%	0.004%
97	14.101	4058	4062	4065	rBV5	2023	1963	0.13%	0.017%
98	14.397	4147	4154	4155	rBV6	1994	2006	0.13%	0.017%
99	14.632	4225	4227	4230	rBV4	1519	480	0.03%	0.004%
100	14.673	4238	4240	4241	rBV2	1288	483	0.03%	0.004%




Sum of corrected areas: 11757756

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032866.D
Acq On : 07 Nov 2023 13:54
Operator : SY/MD
Sample : 05226-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

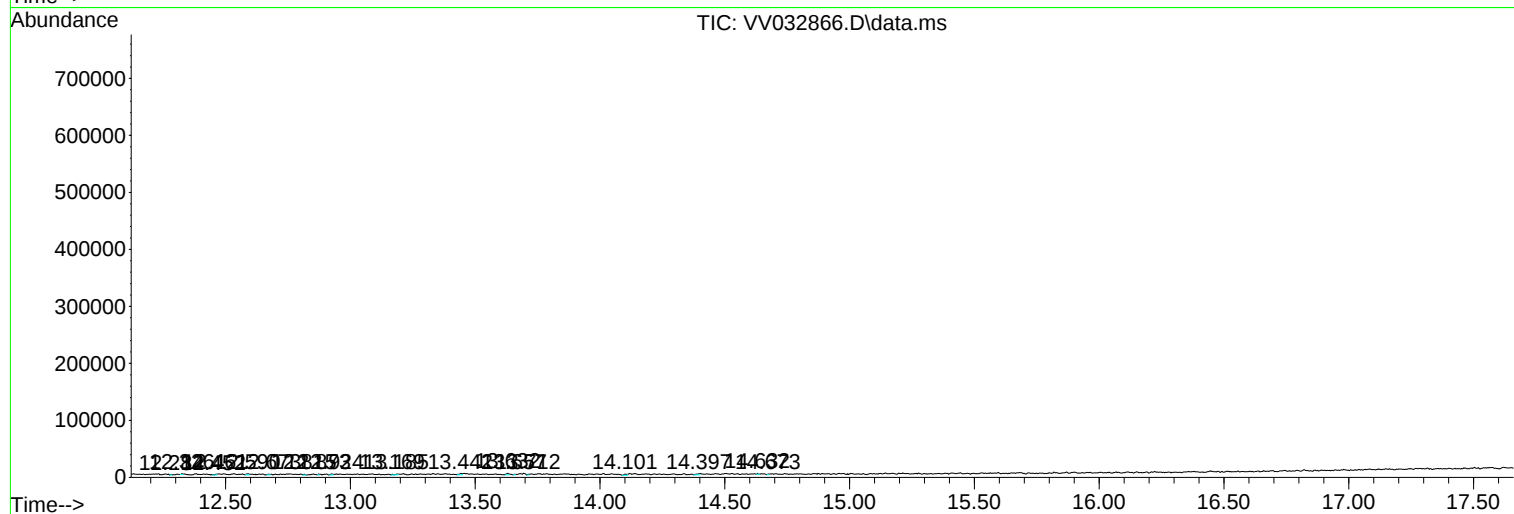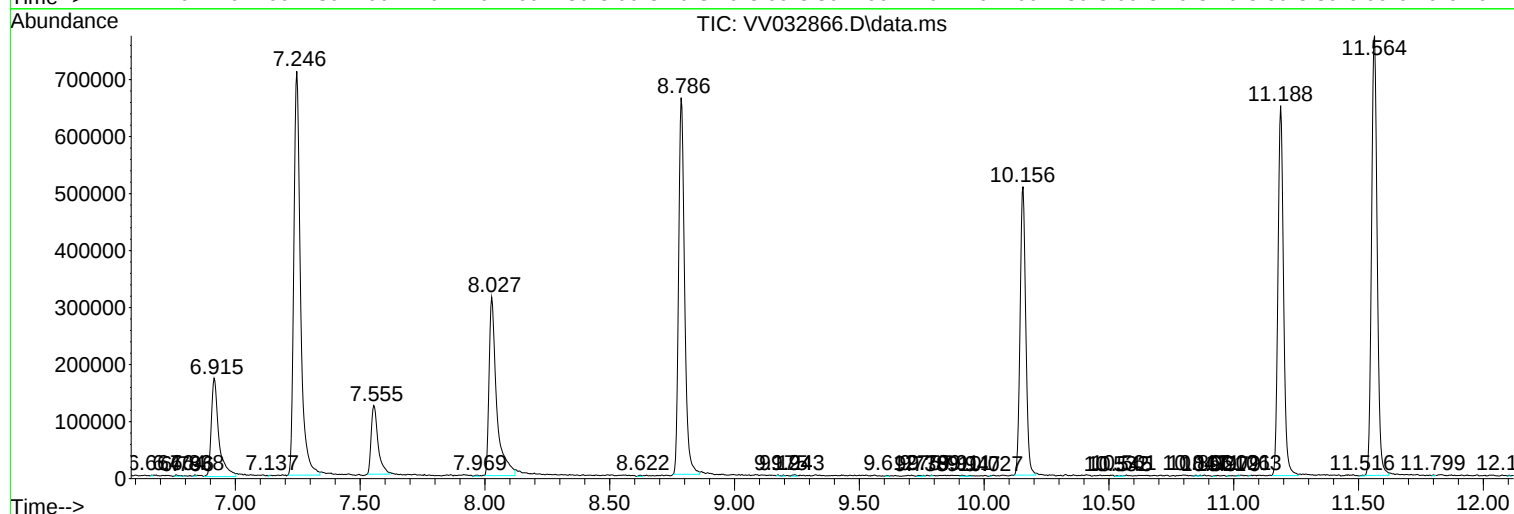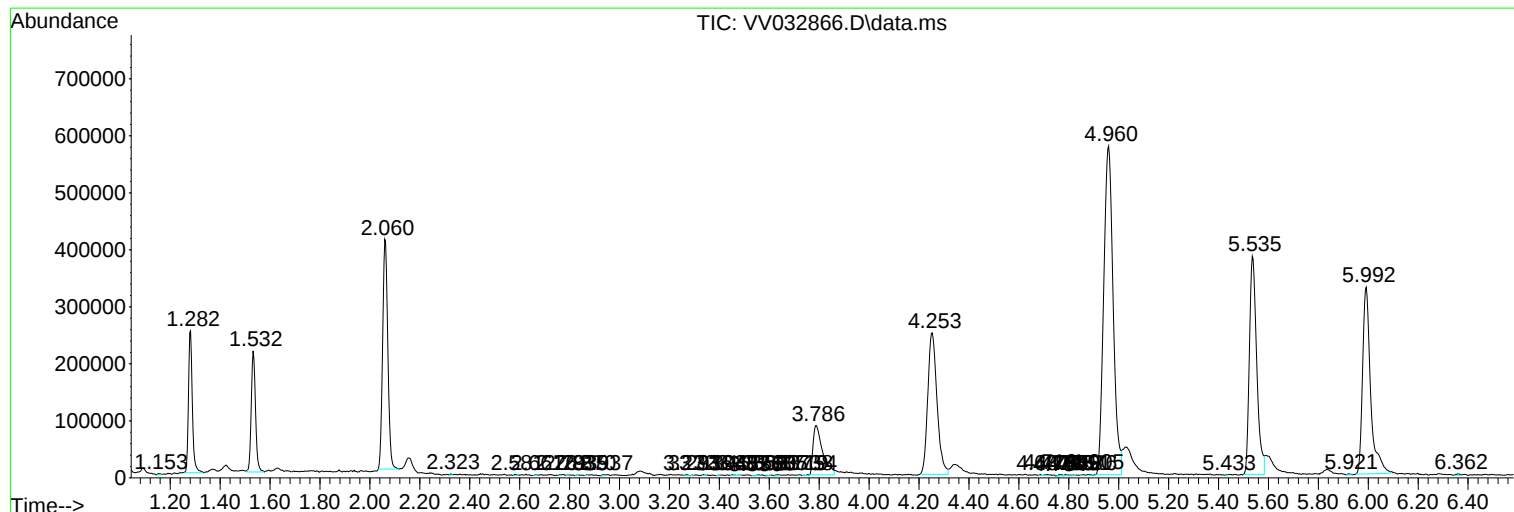

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032866.D
Acq On : 07 Nov 2023 13:54
Operator : SY/MD
Sample : 05226-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032866.D
Acq On : 07 Nov 2023 13:54
Operator : SY/MD
Sample : 05226-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc