

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032867.D
 Acq On : 07 Nov 2023 14:18
 Operator : SY/MD
 Sample : 05226-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	52	56	57	rBV3	3066	2159	0.15%	0.019%
2	1.281	68	75	92	rVB	235966	251947	17.10%	2.178%
3	1.532	146	153	165	rVB	204360	239086	16.23%	2.067%
4	2.060	309	317	337	rVB	401749	579569	39.34%	5.011%
5	2.384	415	418	420	rBV4	1854	1106	0.08%	0.010%
6	2.436	432	434	435	rBV2	1742	748	0.05%	0.006%
7	2.519	458	460	463	rVB3	1839	944	0.06%	0.008%
8	2.574	474	477	480	rVV4	1560	960	0.07%	0.008%
9	2.590	480	482	484	rVB3	1513	646	0.04%	0.006%
10	2.780	538	541	544	rBV5	2519	1792	0.12%	0.015%
11	2.957	591	596	597	rVV4	1499	1047	0.07%	0.009%
12	3.076	628	633	636	rVB7	1851	2053	0.14%	0.018%
13	3.101	636	641	643	rBV6	904	810	0.05%	0.007%
14	3.133	648	651	653	rBV4	1151	607	0.04%	0.005%
15	3.159	657	659	661	rBV3	1600	828	0.06%	0.007%
16	3.175	661	664	666	rBV4	1299	585	0.04%	0.005%
17	3.214	671	676	678	rBV5	1111	989	0.07%	0.009%
18	3.355	718	720	724	rBV4	1302	839	0.06%	0.007%
19	3.420	738	740	745	rBV6	1466	773	0.05%	0.007%
20	3.484	758	760	762	rBV3	1449	709	0.05%	0.006%
21	3.503	764	766	772	rVV6	1743	1376	0.09%	0.012%
22	3.568	784	786	787	rBV2	1246	645	0.04%	0.006%
23	3.587	790	792	793	rVV2	1383	600	0.04%	0.005%
24	3.600	793	796	798	rVV4	1766	976	0.07%	0.008%
25	3.616	798	801	806	rVV6	1141	1105	0.07%	0.010%
26	3.706	825	829	832	rVB6	1664	882	0.06%	0.008%
27	3.789	846	855	880	rBV2	84361	229865	15.60%	1.987%
28	4.252	986	999	1018	rBV2	236993	592513	40.21%	5.123%
29	4.580	1099	1101	1103	rBV3	1960	822	0.06%	0.007%
30	4.677	1126	1131	1135	rVB7	3012	2691	0.18%	0.023%
31	4.699	1135	1138	1140	rBV4	1389	967	0.07%	0.008%
32	4.764	1155	1158	1160	rBV4	1612	1013	0.07%	0.009%
33	4.960	1203	1219	1235	rBV2	559932	1473365	100.00%	12.738%
34	5.355	1338	1342	1348	rBV8	2006	2218	0.15%	0.019%
35	5.449	1367	1371	1372	rBV4	1714	1460	0.10%	0.013%
36	5.535	1387	1398	1413	rBV	379555	783878	53.20%	6.777%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032867.D
 Acq On : 07 Nov 2023 14:18
 Operator : SY/MD
 Sample : 05226-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.992	1528	1540	1572	rBV	321356	722631	49.05%	6.248%
38	6.288	1627	1632	1633	rBV5	2496	1851	0.13%	0.016%
39	6.394	1663	1665	1667	rBV3	1816	833	0.06%	0.007%
40	6.442	1675	1680	1682	rBV4	2623	1603	0.11%	0.014%
41	6.693	1755	1758	1761	rBV5	1314	1222	0.08%	0.011%
42	6.841	1800	1804	1806	rBV5	2398	1400	0.10%	0.012%
43	6.915	1817	1827	1852	rBV	167917	339815	23.06%	2.938%
44	7.175	1903	1908	1911	rBV7	2811	3000	0.20%	0.026%
45	7.246	1919	1930	1960	rBV	693300	1296313	87.98%	11.207%
46	7.555	2018	2026	2047	rBV	120420	223971	15.20%	1.936%
47	8.027	2164	2173	2202	rBV	304551	631049	42.83%	5.456%
48	8.596	2348	2350	2354	rVB5	1676	944	0.06%	0.008%
49	8.722	2387	2389	2390	rBV2	1449	610	0.04%	0.005%
50	8.786	2398	2409	2438	rBV	654420	1128474	76.59%	9.756%
51	9.069	2494	2497	2499	rBV2	1812	1275	0.09%	0.011%
52	9.249	2550	2553	2555	rBV3	2127	1218	0.08%	0.011%
53	9.345	2579	2583	2585	rBV3	2112	1505	0.10%	0.013%
54	9.397	2595	2599	2608	rVB3	2283	3205	0.22%	0.028%
55	9.580	2653	2656	2657	rBV3	1868	877	0.06%	0.008%
56	9.635	2669	2673	2676	rBV5	2025	1842	0.13%	0.016%
57	9.744	2705	2707	2712	rBV6	1317	990	0.07%	0.009%
58	9.821	2728	2731	2733	rBV3	1252	782	0.05%	0.007%
59	9.943	2766	2769	2773	rVB5	1893	1153	0.08%	0.010%
60	9.963	2773	2775	2778	rBV3	1241	821	0.06%	0.007%
61	10.037	2796	2798	2800	rBV3	1032	590	0.04%	0.005%
62	10.114	2819	2822	2824	rBV4	1477	1144	0.08%	0.010%
63	10.156	2824	2835	2859	rVV	489243	780352	52.96%	6.747%
64	10.468	2930	2932	2937	rVB4	1881	1572	0.11%	0.014%
65	10.493	2937	2940	2942	rBV4	2609	1883	0.13%	0.016%
66	10.554	2956	2959	2961	rBV4	1552	737	0.05%	0.006%
67	10.609	2974	2976	2982	rVB7	1361	1419	0.10%	0.012%
68	10.644	2984	2987	2988	rBV3	1382	749	0.05%	0.006%
69	10.734	3010	3015	3021	rBV10	2020	2315	0.16%	0.020%
70	10.828	3042	3044	3050	rVB6	2517	2333	0.16%	0.020%
71	10.873	3052	3058	3062	rBV7	2298	2429	0.16%	0.021%
72	10.982	3090	3092	3096	rVB4	1153	742	0.05%	0.006%
73	11.011	3096	3101	3102	rBV5	1571	1335	0.09%	0.012%
74	11.062	3115	3117	3119	rBV3	1442	991	0.07%	0.009%
75	11.188	3145	3156	3176	rBV	640567	1008562	68.45%	8.720%
76	11.564	3261	3273	3293	rBV	748503	1184734	80.41%	10.243%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032867.D
 Acq On : 07 Nov 2023 14:18
 Operator : SY/MD
 Sample : 05226-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.056	3422	3426	3427	rBV4	1213	719	0.05%	0.006%
78	12.123	3445	3447	3453	rVB6	1911	1155	0.08%	0.010%
79	12.188	3465	3467	3470	rBV4	1265	795	0.05%	0.007%
80	12.249	3484	3486	3489	rBV4	1446	1104	0.07%	0.010%
81	12.406	3533	3535	3537	rBV2	1253	675	0.05%	0.006%
82	12.558	3577	3582	3583	rBV5	1283	1082	0.07%	0.009%
83	12.644	3606	3609	3610	rBV3	1237	690	0.05%	0.006%
84	12.718	3629	3632	3634	rBV4	1285	709	0.05%	0.006%
85	12.741	3638	3639	3641	rBV2	1811	854	0.06%	0.007%
86	12.963	3705	3708	3709	rBV2	1540	798	0.05%	0.007%
87	13.156	3764	3768	3769	rBV4	1204	793	0.05%	0.007%
88	13.207	3780	3784	3787	rBV5	2191	2062	0.14%	0.018%
89	13.291	3807	3810	3812	rBV3	1879	1045	0.07%	0.009%
90	13.336	3820	3824	3825	rBV4	1690	1117	0.08%	0.010%
91	13.583	3898	3901	3904	rBV4	2106	1720	0.12%	0.015%
92	13.673	3927	3929	3932	rBV4	1465	893	0.06%	0.008%
93	13.786	3962	3964	3968	rVB5	2082	1096	0.07%	0.009%
94	13.982	4020	4025	4026	rBV4	1322	1316	0.09%	0.011%
95	14.021	4035	4037	4039	rBV3	1857	733	0.05%	0.006%
96	14.104	4061	4063	4065	rVB3	1951	868	0.06%	0.008%
97	14.127	4065	4070	4072	rBV5	1840	1607	0.11%	0.014%
98	14.162	4079	4081	4085	rBV4	2258	1524	0.10%	0.013%
99	14.210	4094	4096	4098	rBV2	1428	765	0.05%	0.007%
100	14.300	4122	4124	4125	rBV2	2001	626	0.04%	0.005%




Sum of corrected areas: 11566590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032867.D
Acq On : 07 Nov 2023 14:18
Operator : SY/MD
Sample : 05226-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

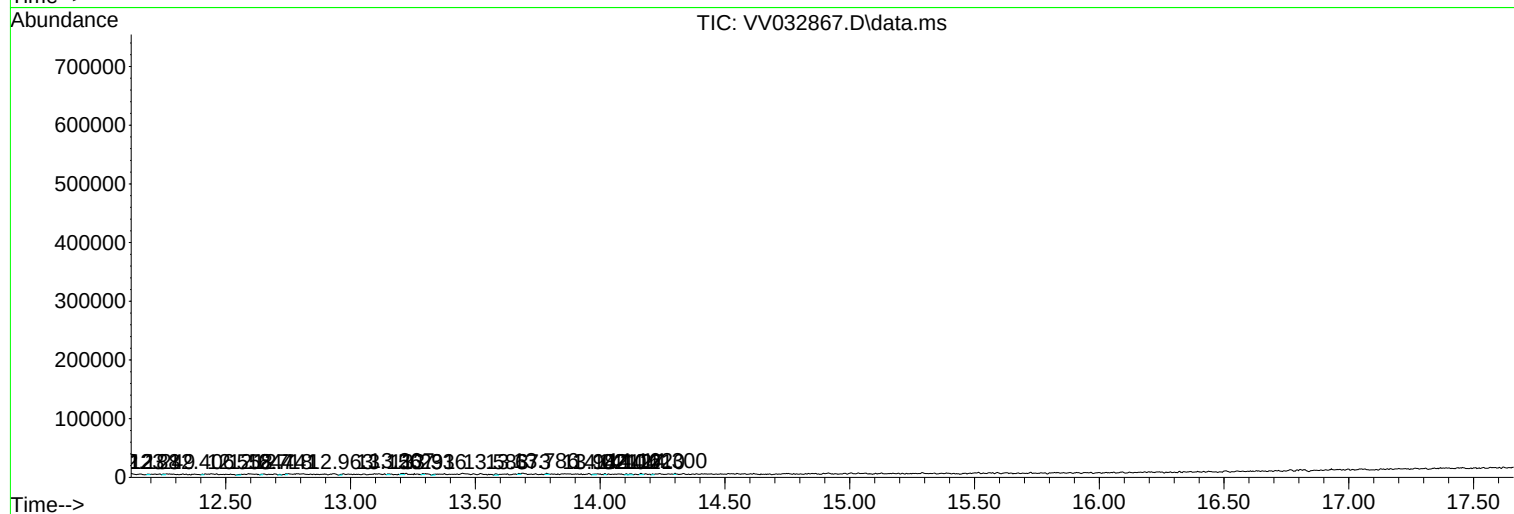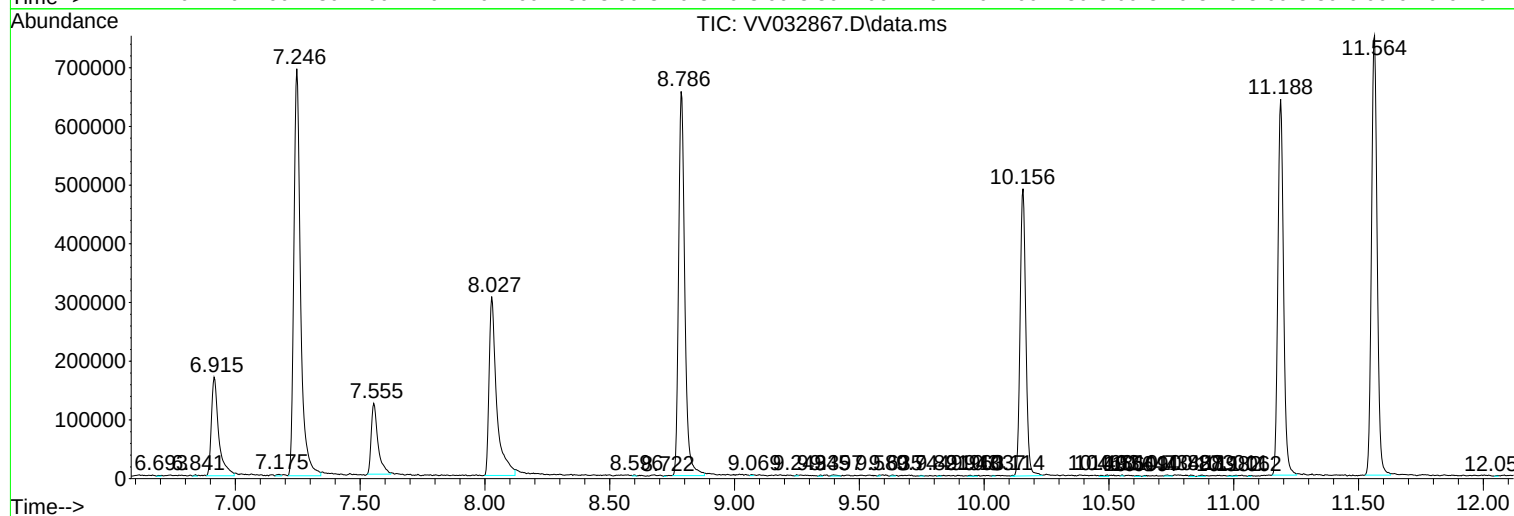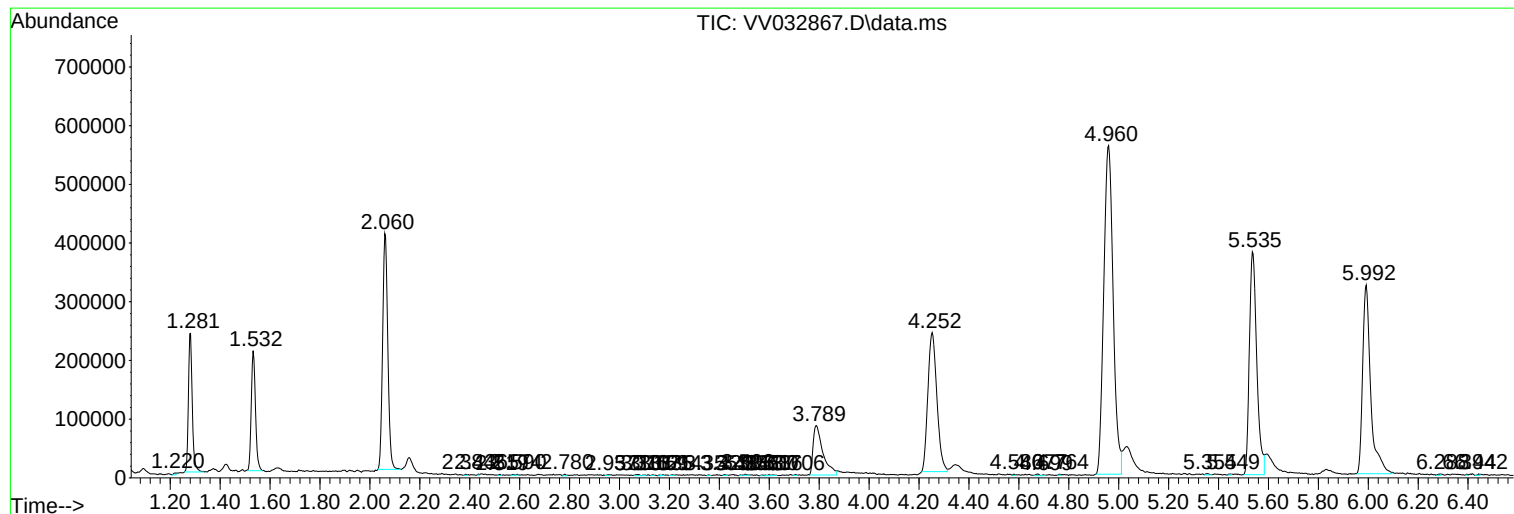

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032867.D
Acq On : 07 Nov 2023 14:18
Operator : SY/MD
Sample : 05226-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032867.D
Acq On : 07 Nov 2023 14:18
Operator : SY/MD
Sample : 05226-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc