

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032868.D
 Acq On : 07 Nov 2023 14:41
 Operator : SY/MD
 Sample : 05226-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rBV	243437	257898	17.28%	2.203%
2	1.532	146	153	167	rVB	214850	250310	16.77%	2.138%
3	2.060	309	317	329	rBV	399450	565609	37.90%	4.831%
4	2.677	507	509	511	rBV2	1249	578	0.04%	0.005%
5	2.870	567	569	571	rBV3	1348	674	0.05%	0.006%
6	2.912	580	582	584	rBV2	1056	495	0.03%	0.004%
7	2.925	584	586	588	rVB3	1603	560	0.04%	0.005%
8	3.008	609	612	616	rVB6	1874	1308	0.09%	0.011%
9	3.034	616	620	621	rBV4	1170	775	0.05%	0.007%
10	3.121	639	647	651	rBV7	1908	3109	0.21%	0.027%
11	3.191	667	669	673	rVB5	1615	923	0.06%	0.008%
12	3.207	673	674	677	rVB3	1673	686	0.05%	0.006%
13	3.230	677	681	683	rBV3	1634	1336	0.09%	0.011%
14	3.265	689	692	693	rBV2	1179	633	0.04%	0.005%
15	3.314	706	707	709	rBV2	1043	575	0.04%	0.005%
16	3.346	713	717	722	rBV7	1948	2135	0.14%	0.018%
17	3.391	729	731	733	rBV3	1364	832	0.06%	0.007%
18	3.580	787	790	792	rBV4	1375	826	0.06%	0.007%
19	3.632	804	806	808	rBV4	1434	812	0.05%	0.007%
20	3.683	816	822	824	rVB7	1452	1227	0.08%	0.010%
21	3.696	824	826	830	rVB5	781	479	0.03%	0.004%
22	3.715	830	832	833	rBV2	1426	648	0.04%	0.006%
23	3.786	845	854	889	rBV	90449	264106	17.70%	2.256%
24	4.185	976	978	982	rVB5	2801	1566	0.10%	0.013%
25	4.252	982	999	1019	rBV	246095	638719	42.80%	5.455%
26	4.558	1092	1094	1096	rBV3	1596	665	0.04%	0.006%
27	4.786	1163	1165	1167	rBV4	1520	854	0.06%	0.007%
28	4.960	1203	1219	1236	rBV2	575402	1492452	100.00%	12.747%
29	5.368	1344	1346	1351	rBV6	1633	1276	0.09%	0.011%
30	5.426	1358	1364	1366	rBV6	2270	2372	0.16%	0.020%
31	5.539	1387	1399	1414	rBV	384523	803187	53.82%	6.860%
32	5.838	1484	1492	1502	rVB7	10809	20600	1.38%	0.176%
33	5.992	1526	1540	1555	rBV	327301	686604	46.01%	5.864%
34	6.407	1667	1669	1672	rVB4	2400	1449	0.10%	0.012%
35	6.426	1672	1675	1676	rBV3	1669	754	0.05%	0.006%
36	6.468	1687	1688	1690	rVB2	2050	615	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032868.D
 Acq On : 07 Nov 2023 14:41
 Operator : SY/MD
 Sample : 05226-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.526	1702	1706	1708	rBV5	2399	1984	0.13%	0.017%
38	6.580	1720	1723	1725	rBV3	1468	1079	0.07%	0.009%
39	6.635	1738	1740	1742	rBV3	954	494	0.03%	0.004%
40	6.747	1772	1775	1776	rBV3	1183	781	0.05%	0.007%
41	6.789	1785	1788	1790	rBV4	1655	1134	0.08%	0.010%
42	6.831	1796	1801	1805	rBV6	2229	2136	0.14%	0.018%
43	6.915	1817	1827	1855	rBV	162490	338019	22.65%	2.887%
44	7.130	1890	1894	1897	rBV5	2399	2243	0.15%	0.019%
45	7.246	1919	1930	1961	rBV	681606	1274718	85.41%	10.887%
46	7.555	2017	2026	2048	rBV	121851	234814	15.73%	2.006%
47	7.879	2125	2127	2132	rBV6	1667	1323	0.09%	0.011%
48	8.027	2164	2173	2208	rBV	317473	669479	44.86%	5.718%
49	8.397	2284	2288	2289	rBV4	1704	1010	0.07%	0.009%
50	8.513	2320	2324	2327	rBV6	2381	1888	0.13%	0.016%
51	8.786	2399	2409	2427	rBV	670332	1130189	75.73%	9.653%
52	9.455	2615	2617	2619	rBV3	1215	514	0.03%	0.004%
53	9.481	2621	2625	2627	rVV4	1612	1277	0.09%	0.011%
54	9.522	2632	2638	2639	rBV5	1698	1473	0.10%	0.013%
55	9.587	2656	2658	2661	rVB4	1034	516	0.03%	0.004%
56	9.612	2664	2666	2671	rVB6	1425	985	0.07%	0.008%
57	9.725	2698	2701	2705	rBV5	1608	1211	0.08%	0.010%
58	9.744	2705	2707	2709	rBV3	1768	876	0.06%	0.007%
59	9.889	2745	2752	2753	rBV6	1822	2308	0.15%	0.020%
60	9.972	2775	2778	2783	rVB6	2259	1649	0.11%	0.014%
61	10.037	2796	2798	2800	rBV3	1526	929	0.06%	0.008%
62	10.082	2807	2812	2813	rBV5	1560	1046	0.07%	0.009%
63	10.156	2824	2835	2850	rBV	490591	775633	51.97%	6.625%
64	10.316	2882	2885	2886	rBV3	1685	1109	0.07%	0.009%
65	10.349	2893	2895	2898	rBV4	1460	932	0.06%	0.008%
66	10.390	2903	2908	2911	rBV6	2071	2323	0.16%	0.020%
67	10.426	2917	2919	2924	rBV5	1315	1333	0.09%	0.011%
68	10.477	2933	2935	2937	rVB3	1885	603	0.04%	0.005%
69	10.551	2954	2958	2960	rBV5	2241	1492	0.10%	0.013%
70	10.590	2967	2970	2974	rBV6	1595	1302	0.09%	0.011%
71	10.754	3019	3021	3024	rBV4	930	601	0.04%	0.005%
72	10.776	3024	3028	3032	rVV6	1913	1796	0.12%	0.015%
73	10.792	3032	3033	3041	rVV7	1813	1718	0.12%	0.015%
74	10.828	3041	3044	3045	rVV3	890	468	0.03%	0.004%
75	10.976	3086	3090	3092	rBV5	2471	1680	0.11%	0.014%
76	11.069	3112	3119	3120	rBV7	2905	2543	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032868.D
 Acq On : 07 Nov 2023 14:41
 Operator : SY/MD
 Sample : 05226-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.188	3145	3156	3173	rBV	665274	1017851	68.20%	8.693%
78	11.564	3261	3273	3290	rBV	752212	1183414	79.29%	10.107%
79	12.091	3434	3437	3439	rBV4	1757	1062	0.07%	0.009%
80	12.169	3459	3461	3462	rBV2	1245	626	0.04%	0.005%
81	12.201	3468	3471	3474	rBV4	2085	1451	0.10%	0.012%
82	12.355	3517	3519	3521	rBV3	1029	655	0.04%	0.006%
83	12.384	3526	3528	3530	rVB3	1667	637	0.04%	0.005%
84	12.651	3608	3611	3613	rBV5	1905	1287	0.09%	0.011%
85	12.686	3618	3622	3623	rBV4	1657	1040	0.07%	0.009%
86	12.828	3660	3666	3673	rBV4	2409	3703	0.25%	0.032%
87	13.053	3731	3736	3738	rBV5	1378	1426	0.10%	0.012%
88	13.284	3805	3808	3811	rBV4	2334	1569	0.11%	0.013%
89	13.310	3814	3816	3819	rVB3	1996	1250	0.08%	0.011%
90	13.358	3829	3831	3833	rVB3	2683	1157	0.08%	0.010%
91	13.381	3833	3838	3841	rBV6	2406	2278	0.15%	0.019%
92	13.596	3901	3905	3906	rBV4	1841	1077	0.07%	0.009%
93	13.660	3923	3925	3927	rVB3	1412	529	0.04%	0.005%
94	13.885	3989	3995	3997	rBV6	2413	2370	0.16%	0.020%
95	14.008	4029	4033	4037	rVB5	1907	1689	0.11%	0.014%
96	14.040	4040	4043	4045	rBV4	2133	1144	0.08%	0.010%
97	14.066	4047	4051	4052	rBV4	2330	1414	0.09%	0.012%
98	14.133	4066	4072	4076	rBV8	2220	2812	0.19%	0.024%
99	14.342	4135	4137	4139	rVB3	1839	759	0.05%	0.006%
100	14.715	4248	4253	4254	rBV5	2785	1909	0.13%	0.016%




Sum of corrected areas: 11708364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032868.D
Acq On : 07 Nov 2023 14:41
Operator : SY/MD
Sample : 05226-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

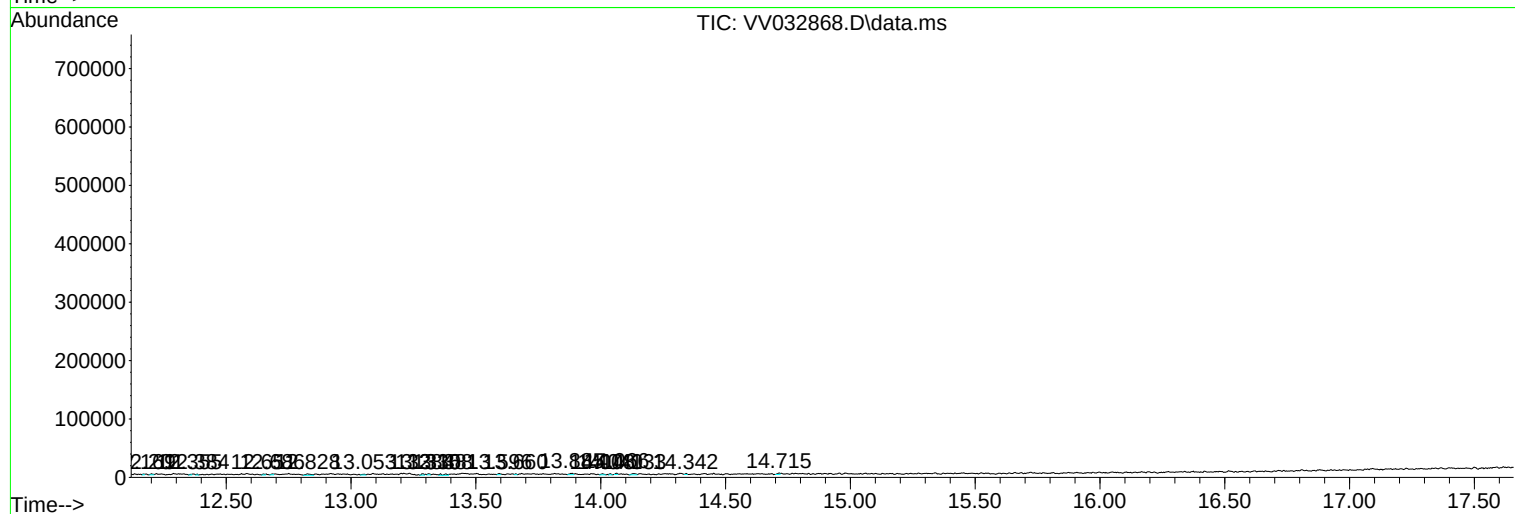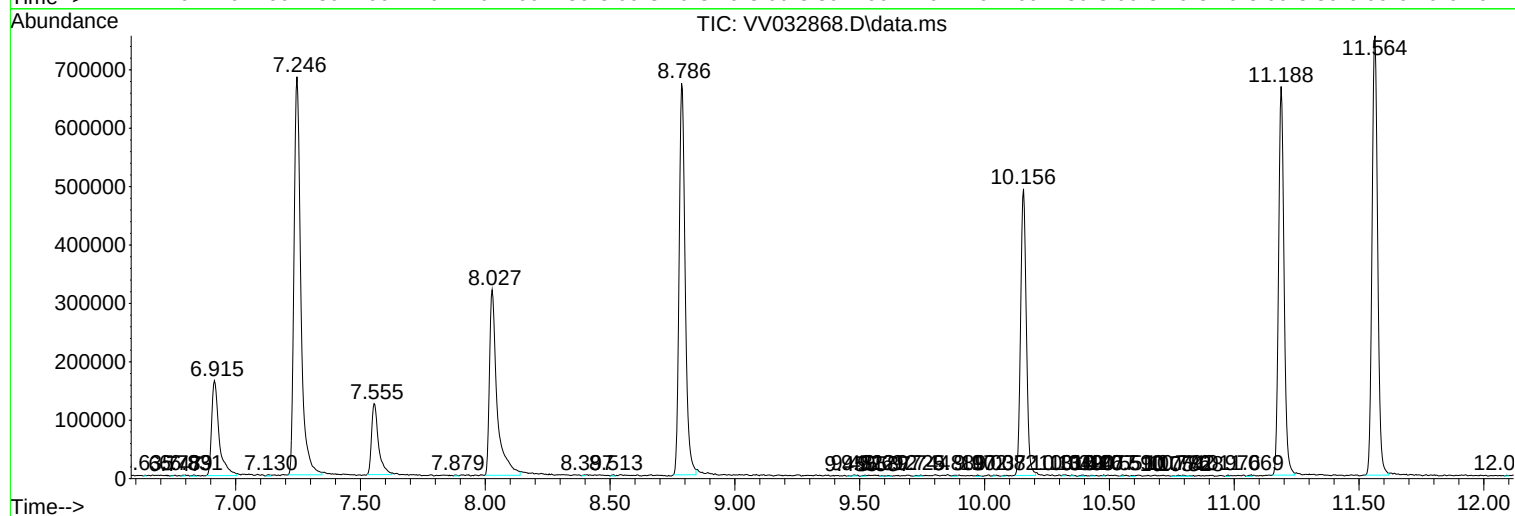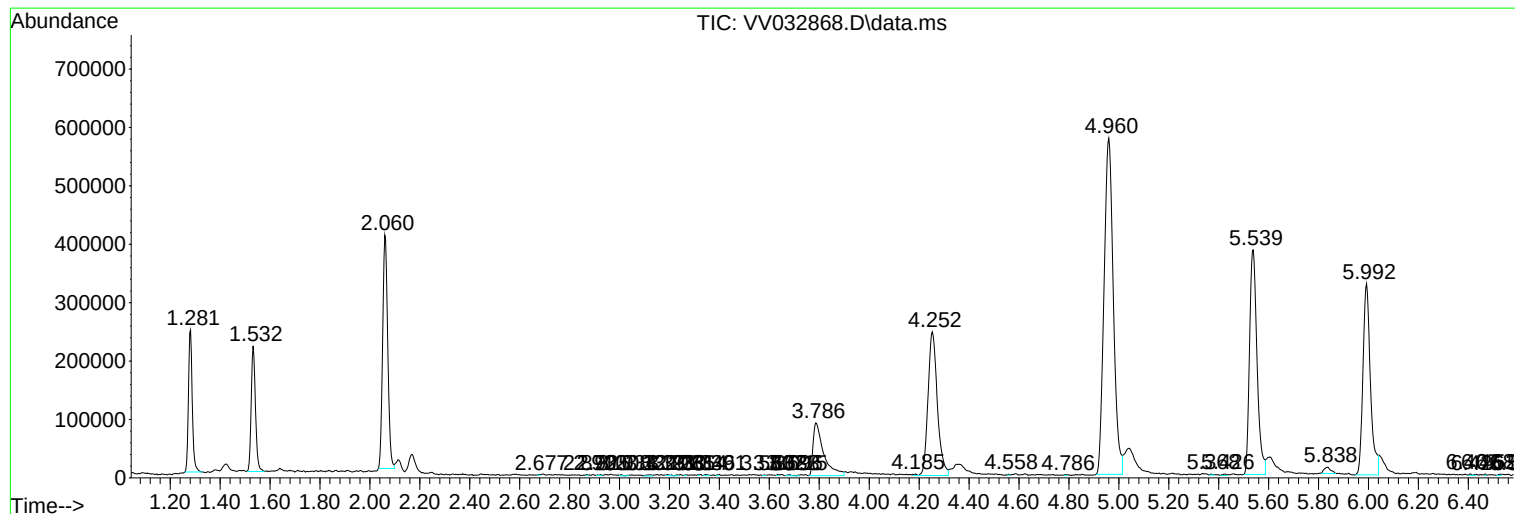

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032868.D
Acq On : 07 Nov 2023 14:41
Operator : SY/MD
Sample : 05226-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032868.D
Acq On : 07 Nov 2023 14:41
Operator : SY/MD
Sample : 05226-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------