

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032869.D
 Acq On : 07 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05226-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rBV	257393	266038	17.76%	2.274%
2	1.532	146	153	165	rVB	210410	244510	16.32%	2.090%
3	2.060	309	317	333	rBV	394074	570362	38.07%	4.874%
4	2.330	399	401	404	rBV4	1369	972	0.06%	0.008%
5	2.548	466	469	472	rBV5	3078	2536	0.17%	0.022%
6	2.587	477	481	483	rVV4	1553	845	0.06%	0.007%
7	2.770	537	538	540	rVB2	1976	628	0.04%	0.005%
8	2.822	551	554	556	rBV4	1213	680	0.05%	0.006%
9	2.854	562	564	565	rBV2	1194	491	0.03%	0.004%
10	2.912	578	582	584	rBV5	1195	863	0.06%	0.007%
11	2.973	596	601	604	rVB7	2183	1791	0.12%	0.015%
12	2.992	604	607	611	rBV6	1497	1358	0.09%	0.012%
13	3.014	611	614	615	rBV2	1119	447	0.03%	0.004%
14	3.069	628	631	633	rBV4	1266	822	0.05%	0.007%
15	3.114	643	645	646	rBV2	1266	491	0.03%	0.004%
16	3.191	667	669	670	rBV2	881	420	0.03%	0.004%
17	3.256	686	689	691	rBV4	1446	929	0.06%	0.008%
18	3.278	695	696	700	rVB4	1142	475	0.03%	0.004%
19	3.368	721	724	727	rBV5	1334	972	0.06%	0.008%
20	3.407	734	736	739	rBV4	2197	1391	0.09%	0.012%
21	3.484	756	760	762	rBV4	1360	861	0.06%	0.007%
22	3.529	771	774	775	rBV3	2104	1101	0.07%	0.009%
23	3.558	781	783	785	rVB3	1491	740	0.05%	0.006%
24	3.619	800	802	804	rVB3	1229	485	0.03%	0.004%
25	3.638	804	808	810	rBV5	1251	1007	0.07%	0.009%
26	3.712	829	831	835	rBV5	1210	895	0.06%	0.008%
27	3.741	839	840	844	rVB4	1031	458	0.03%	0.004%
28	3.789	844	855	885	rBV	92527	263500	17.59%	2.252%
29	4.146	961	966	969	rBV7	2170	1995	0.13%	0.017%
30	4.252	986	999	1020	rBV2	236329	597617	39.89%	5.107%
31	4.577	1097	1100	1104	rBV5	2208	1995	0.13%	0.017%
32	4.757	1152	1156	1160	rBV7	1629	1607	0.11%	0.014%
33	4.818	1172	1175	1176	rBV3	1512	671	0.04%	0.006%
34	4.841	1179	1182	1185	rBV5	1056	796	0.05%	0.007%
35	4.960	1202	1219	1236	rBV2	571322	1498246	100.00%	12.804%
36	5.538	1387	1399	1414	rBV	378832	788214	52.61%	6.736%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032869.D
 Acq On : 07 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05226-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.992	1528	1540	1572	rBV	326993	730708	48.77%	6.245%
38	6.436	1676	1678	1681	rBV4	1199	808	0.05%	0.007%
39	6.577	1720	1722	1728	rVB6	1765	1673	0.11%	0.014%
40	6.735	1769	1771	1774	rBV4	1111	444	0.03%	0.004%
41	6.796	1787	1790	1791	rBV2	1608	750	0.05%	0.006%
42	6.825	1797	1799	1801	rBV3	1183	516	0.03%	0.004%
43	6.915	1816	1827	1853	rBV	170353	346519	23.13%	2.961%
44	7.246	1919	1930	1967	rBV	693934	1288902	86.03%	11.015%
45	7.554	2018	2026	2048	rBV	122667	224672	15.00%	1.920%
46	7.847	2115	2117	2119	rVB4	1392	421	0.03%	0.004%
47	8.027	2164	2173	2210	rBV	323643	690320	46.08%	5.900%
48	8.429	2296	2298	2299	rBV2	1285	529	0.04%	0.005%
49	8.474	2309	2312	2313	rBV3	1971	1092	0.07%	0.009%
50	8.731	2389	2392	2394	rBV4	1212	858	0.06%	0.007%
51	8.786	2398	2409	2435	rBV	655786	1126754	75.20%	9.629%
52	9.271	2557	2560	2563	rBV4	1571	1341	0.09%	0.011%
53	9.445	2611	2614	2616	rBV3	1801	1275	0.09%	0.011%
54	9.493	2626	2629	2630	rBV3	2255	1180	0.08%	0.010%
55	9.651	2675	2678	2679	rBV3	1327	790	0.05%	0.007%
56	9.757	2709	2711	2712	rBV2	1459	613	0.04%	0.005%
57	9.866	2744	2745	2750	rBV5	1217	1181	0.08%	0.010%
58	9.998	2783	2786	2788	rBV4	1143	801	0.05%	0.007%
59	10.059	2801	2805	2809	rBV7	1676	1628	0.11%	0.014%
60	10.156	2824	2835	2857	rVB	490264	772585	51.57%	6.603%
61	10.333	2888	2890	2896	rVB7	1772	1150	0.08%	0.010%
62	10.445	2923	2925	2927	rBV3	1330	792	0.05%	0.007%
63	10.583	2965	2968	2972	rBV5	1489	1230	0.08%	0.011%
64	10.638	2983	2985	2987	rBV3	1153	593	0.04%	0.005%
65	10.677	2995	2997	2998	rBV2	1323	402	0.03%	0.003%
66	10.776	3024	3028	3029	rBV3	1025	712	0.05%	0.006%
67	10.853	3050	3052	3054	rBV3	1379	736	0.05%	0.006%
68	10.927	3073	3075	3078	rBV3	1102	846	0.06%	0.007%
69	10.992	3093	3095	3098	rVB3	1469	628	0.04%	0.005%
70	11.075	3119	3121	3122	rBV2	1106	429	0.03%	0.004%
71	11.095	3125	3127	3129	rBV3	1684	848	0.06%	0.007%
72	11.188	3145	3156	3180	rBV	652727	1015790	67.80%	8.681%
73	11.564	3261	3273	3291	rBV	755828	1198294	79.98%	10.241%
74	11.924	3383	3385	3386	rBV2	1460	619	0.04%	0.005%
75	11.976	3400	3401	3403	rVB2	1733	560	0.04%	0.005%
76	11.992	3403	3406	3408	rBB4	1147	576	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032869.D
 Acq On : 07 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05226-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.004	3408	3410	3412	rBV2	958	525	0.04%	0.004%
78	12.133	3447	3450	3455	rBV7	1814	1115	0.07%	0.010%
79	12.429	3541	3542	3543	rBV	1432	387	0.03%	0.003%
80	12.567	3583	3585	3588	rBV4	1345	918	0.06%	0.008%
81	12.628	3602	3604	3607	rBV4	1758	975	0.07%	0.008%
82	12.763	3642	3646	3648	rBV5	1640	1458	0.10%	0.012%
83	12.802	3653	3658	3661	rBV7	2409	1854	0.12%	0.016%
84	12.863	3675	3677	3679	rBV4	1921	990	0.07%	0.008%
85	13.011	3720	3723	3725	rBV4	1028	697	0.05%	0.006%
86	13.156	3765	3768	3770	rBV4	2041	1174	0.08%	0.010%
87	13.207	3781	3784	3786	rBV4	2256	1524	0.10%	0.013%
88	13.265	3799	3802	3804	rBV4	1340	1012	0.07%	0.009%
89	13.316	3816	3818	3822	rBV5	911	413	0.03%	0.004%
90	13.516	3879	3880	3882	rVB	1153	360	0.02%	0.003%
91	13.619	3910	3912	3915	rBV4	1913	776	0.05%	0.007%
92	13.670	3926	3928	3930	rBV2	1462	632	0.04%	0.005%
93	13.686	3930	3933	3939	rVV8	2574	2448	0.16%	0.021%
94	13.898	3997	3999	4001	rBV3	2507	1098	0.07%	0.009%
95	13.937	4008	4011	4013	rBV5	2105	1485	0.10%	0.013%
96	14.085	4053	4057	4058	rBV3	1536	877	0.06%	0.007%
97	14.136	4071	4073	4074	rBV2	1328	539	0.04%	0.005%
98	14.268	4112	4114	4116	rBV3	1831	961	0.06%	0.008%
99	14.516	4189	4191	4192	rBV2	1270	486	0.03%	0.004%
100	14.863	4297	4299	4300	rBV3	1756	622	0.04%	0.005%




Sum of corrected areas: 11701100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032869.D
Acq On : 07 Nov 2023 15:04
Operator : SY/MD
Sample : 05226-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

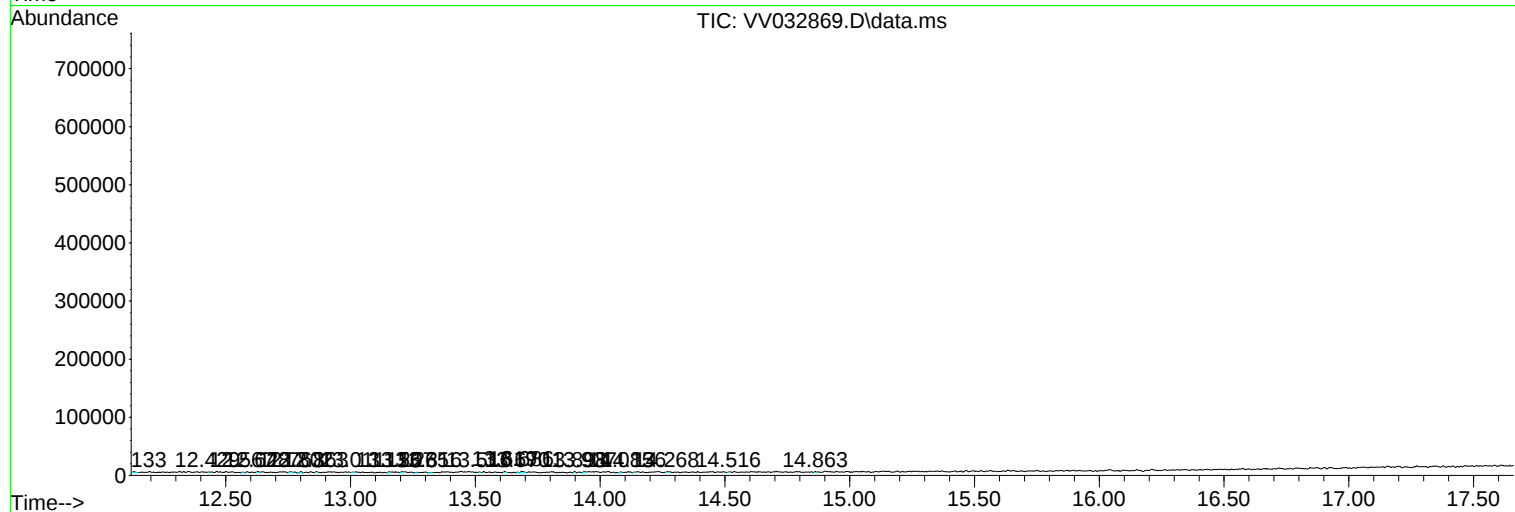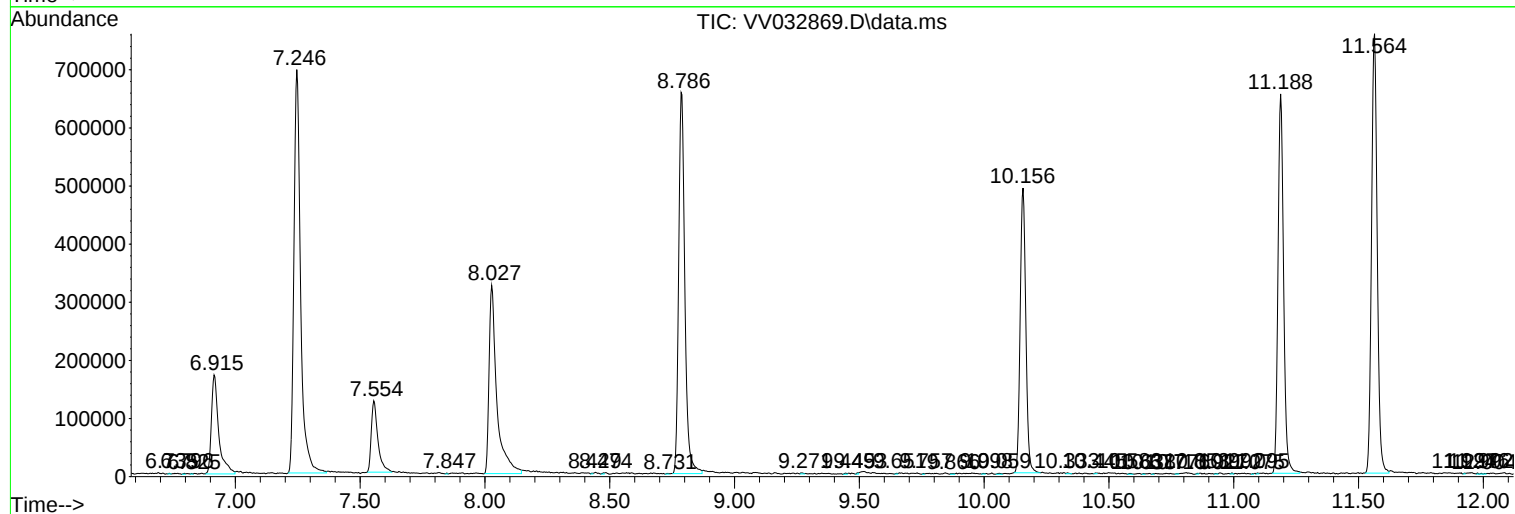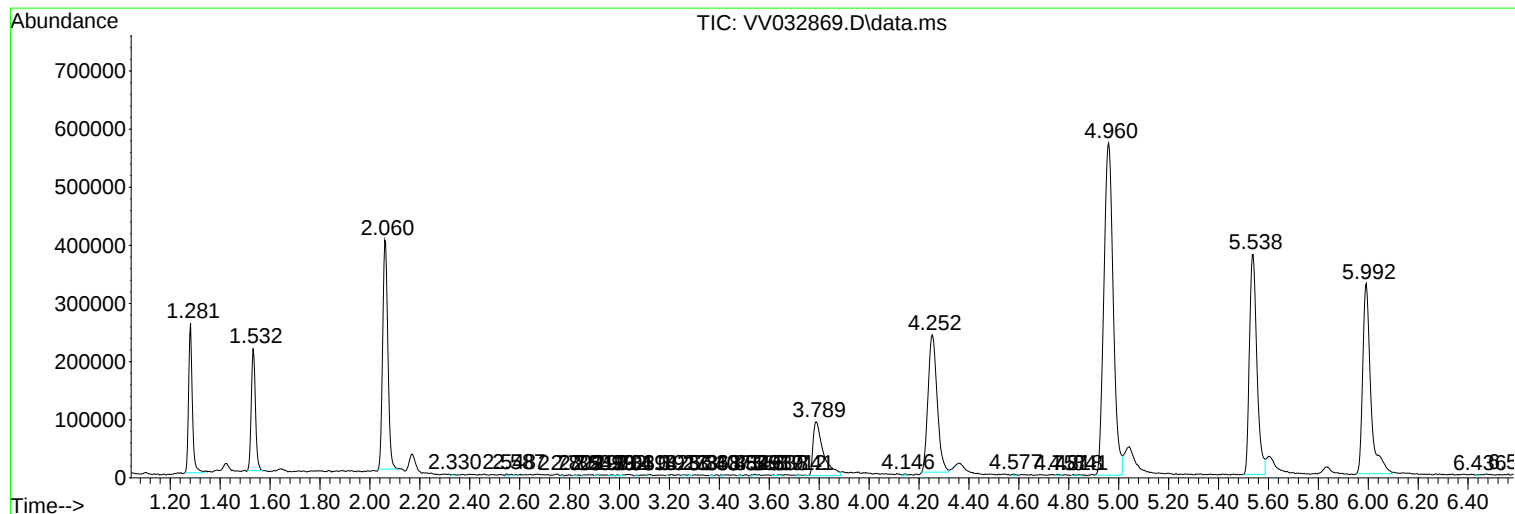

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032869.D
Acq On : 07 Nov 2023 15:04
Operator : SY/MD
Sample : 05226-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032869.D
Acq On : 07 Nov 2023 15:04
Operator : SY/MD
Sample : 05226-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc