

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032870.D
 Acq On : 07 Nov 2023 15:28
 Operator : SY/MD
 Sample : 05226-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	243273	256845	17.32%	2.237%
2	1.532	147	153	171	rVB	209585	243513	16.42%	2.121%
3	2.063	309	318	329	rBV	388677	559428	37.73%	4.873%
4	2.381	416	417	418	rBV2	1320	414	0.03%	0.004%
5	2.420	425	429	430	rBV3	1453	1045	0.07%	0.009%
6	2.600	482	485	489	rBV5	2126	1578	0.11%	0.014%
7	2.670	505	507	509	rBV2	1334	491	0.03%	0.004%
8	2.735	525	527	529	rBV3	757	290	0.02%	0.003%
9	2.789	540	544	548	rVB7	1861	1435	0.10%	0.013%
10	2.809	548	550	552	rBV3	623	405	0.03%	0.004%
11	2.818	552	553	556	rVB3	1159	587	0.04%	0.005%
12	2.834	556	558	559	rBV3	974	403	0.03%	0.004%
13	2.883	570	573	575	rVB4	2389	1384	0.09%	0.012%
14	2.905	577	580	583	rBV4	1326	935	0.06%	0.008%
15	2.992	605	607	608	rBV3	810	285	0.02%	0.002%
16	3.024	616	617	619	rBV2	1169	583	0.04%	0.005%
17	3.088	634	637	640	rBV5	2292	1891	0.13%	0.016%
18	3.140	650	653	656	rVB4	1561	871	0.06%	0.008%
19	3.166	656	661	663	rVB5	1785	1256	0.08%	0.011%
20	3.182	663	666	667	rBV3	1670	918	0.06%	0.008%
21	3.217	673	677	679	rBV5	1445	1112	0.08%	0.010%
22	3.259	686	690	692	rVB5	1636	971	0.07%	0.008%
23	3.342	712	716	717	rBV3	643	447	0.03%	0.004%
24	3.423	738	741	742	rBV2	829	402	0.03%	0.004%
25	3.481	757	759	761	rBV2	801	389	0.03%	0.003%
26	3.503	761	766	769	rVV6	1823	1361	0.09%	0.012%
27	3.519	769	771	775	rVV4	1622	987	0.07%	0.009%
28	3.587	790	792	797	rVB6	1344	1263	0.09%	0.011%
29	3.677	817	820	821	rBV2	1431	648	0.04%	0.006%
30	3.789	846	855	883	rBV2	88183	240070	16.19%	2.091%
31	4.104	950	953	956	rBV5	1635	1367	0.09%	0.012%
32	4.185	971	978	979	rBV6	1796	1904	0.13%	0.017%
33	4.252	984	999	1022	rBV	236605	622913	42.01%	5.426%
34	4.526	1082	1084	1086	rBV4	1402	919	0.06%	0.008%
35	4.632	1116	1117	1120	rVB3	789	349	0.02%	0.003%
36	4.828	1176	1178	1180	rBV3	788	485	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032870.D
 Acq On : 07 Nov 2023 15:28
 Operator : SY/MD
 Sample : 05226-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.889	1195	1197	1199	rBV3	1681	892	0.06%	0.008%
38	4.960	1203	1219	1236	rBV2	573344	1482623	100.00%	12.915%
39	5.539	1387	1399	1415	rBV	378322	779326	52.56%	6.789%
40	5.992	1528	1540	1554	rBV	322514	663664	44.76%	5.781%
41	6.349	1648	1651	1654	rBV5	2109	1510	0.10%	0.013%
42	6.365	1654	1656	1659	rVV4	1391	1025	0.07%	0.009%
43	6.465	1685	1687	1689	rBV3	1547	905	0.06%	0.008%
44	6.735	1769	1771	1773	rBV3	1392	620	0.04%	0.005%
45	6.780	1782	1785	1788	rBV4	1816	1291	0.09%	0.011%
46	6.915	1818	1827	1854	rBV	163587	330313	22.28%	2.877%
47	7.246	1918	1930	1961	rBV	687397	1287929	86.87%	11.219%
48	7.555	2018	2026	2050	rBV	118434	222174	14.99%	1.935%
49	8.027	2164	2173	2204	rBV	310848	663441	44.75%	5.779%
50	8.497	2316	2319	2323	rBV5	2046	1739	0.12%	0.015%
51	8.561	2336	2339	2341	rBV4	1876	1012	0.07%	0.009%
52	8.654	2367	2368	2370	rBV2	988	369	0.02%	0.003%
53	8.747	2394	2397	2398	rBV2	1585	782	0.05%	0.007%
54	8.786	2399	2409	2433	rVV	644105	1096740	73.97%	9.554%
55	9.236	2547	2549	2553	rVB5	1785	1253	0.08%	0.011%
56	9.352	2580	2585	2588	rBV5	1607	1893	0.13%	0.016%
57	9.452	2614	2616	2618	rBV3	1133	487	0.03%	0.004%
58	9.497	2626	2630	2631	rBV4	2837	1850	0.12%	0.016%
59	9.596	2659	2661	2663	rBV3	1236	609	0.04%	0.005%
60	9.609	2663	2665	2667	rBV3	1475	735	0.05%	0.006%
61	9.870	2744	2746	2747	rBV2	1091	461	0.03%	0.004%
62	9.956	2771	2773	2775	rBV3	1630	683	0.05%	0.006%
63	10.091	2813	2815	2819	rVB5	1691	1137	0.08%	0.010%
64	10.156	2824	2835	2852	rVV	485684	766756	51.72%	6.679%
65	10.525	2948	2950	2954	rVB5	1574	782	0.05%	0.007%
66	10.561	2960	2961	2963	rBV2	791	421	0.03%	0.004%
67	10.625	2977	2981	2983	rBV4	2147	1640	0.11%	0.014%
68	10.648	2986	2988	2992	rVV4	1774	1292	0.09%	0.011%
69	10.876	3057	3059	3062	rBV3	1814	955	0.06%	0.008%
70	10.995	3094	3096	3099	rBV4	1540	990	0.07%	0.009%
71	11.062	3112	3117	3119	rBV4	2280	2106	0.14%	0.018%
72	11.188	3145	3156	3177	rBV	638328	993825	67.03%	8.657%
73	11.519	3257	3259	3260	rBV2	1442	334	0.02%	0.003%
74	11.564	3260	3273	3291	rBV	753737	1186565	80.03%	10.336%
75	11.779	3336	3340	3344	rBV6	1832	1587	0.11%	0.014%
76	11.960	3393	3396	3399	rVB5	1872	1128	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032870.D
 Acq On : 07 Nov 2023 15:28
 Operator : SY/MD
 Sample : 05226-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.062	3425	3428	3430	rBV4	1150	639	0.04%	0.006%
78	12.230	3474	3480	3481	rBV6	1818	1832	0.12%	0.016%
79	12.394	3528	3531	3533	rBV3	2073	1439	0.10%	0.013%
80	12.455	3546	3550	3553	rBV6	1224	1150	0.08%	0.010%
81	12.480	3553	3558	3560	rVB5	1790	1447	0.10%	0.013%
82	12.503	3561	3565	3567	rBV5	1762	1204	0.08%	0.010%
83	12.651	3609	3611	3614	rBV4	1796	1041	0.07%	0.009%
84	12.767	3644	3647	3649	rBV4	2321	1275	0.09%	0.011%
85	12.947	3700	3703	3705	rBV4	2231	1213	0.08%	0.011%
86	13.111	3751	3754	3758	rVB5	1836	1214	0.08%	0.011%
87	13.133	3758	3761	3764	rBV6	2954	2206	0.15%	0.019%
88	13.194	3776	3780	3781	rBV5	1362	981	0.07%	0.009%
89	13.403	3843	3845	3847	rBV3	978	481	0.03%	0.004%
90	13.541	3886	3888	3891	rBV4	2027	1464	0.10%	0.013%
91	13.725	3943	3945	3948	rBV4	1139	648	0.04%	0.006%
92	13.808	3969	3971	3972	rBV	1700	756	0.05%	0.007%
93	13.869	3989	3990	3991	rBV	1151	386	0.03%	0.003%
94	13.950	4013	4015	4016	rBV2	1617	517	0.03%	0.005%
95	14.001	4030	4031	4032	rBV	1141	332	0.02%	0.003%
96	14.043	4042	4044	4045	rBV2	1539	441	0.03%	0.004%
97	14.149	4074	4077	4079	rBV4	1623	1168	0.08%	0.010%
98	14.226	4099	4101	4105	rBV4	1720	1152	0.08%	0.010%
99	15.027	4348	4350	4351	rBV2	2185	946	0.06%	0.008%
100	15.545	4509	4511	4515	rBV4	2232	1845	0.12%	0.016%




Sum of corrected areas: 11479765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032870.D
Acq On : 07 Nov 2023 15:28
Operator : SY/MD
Sample : 05226-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

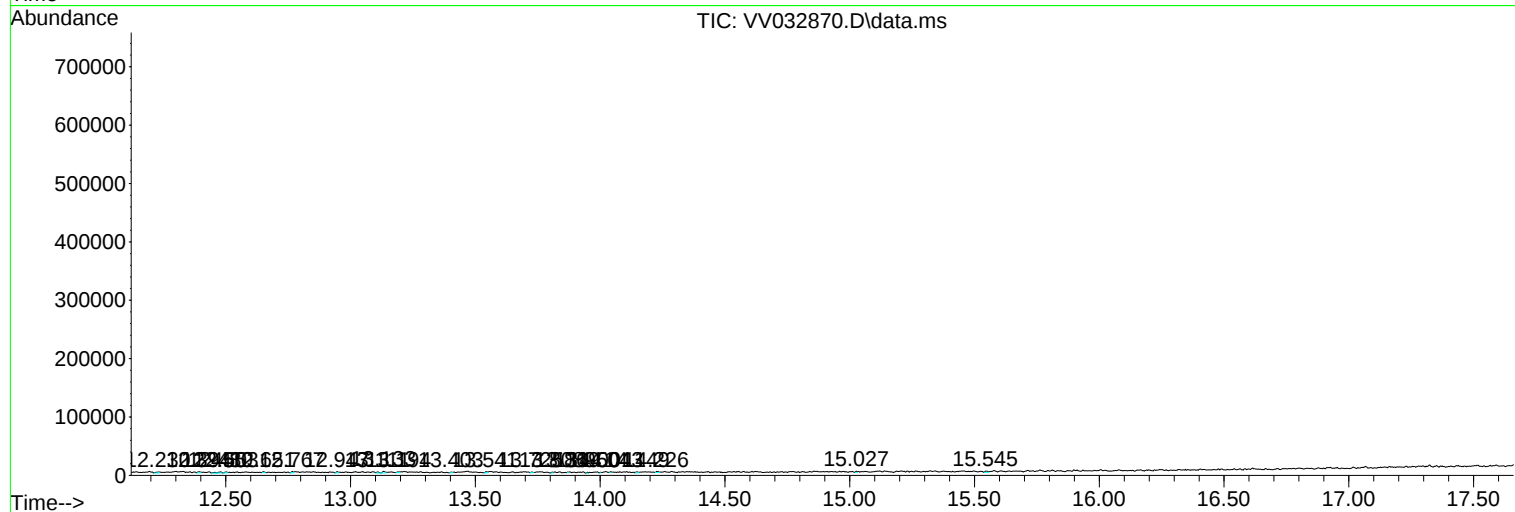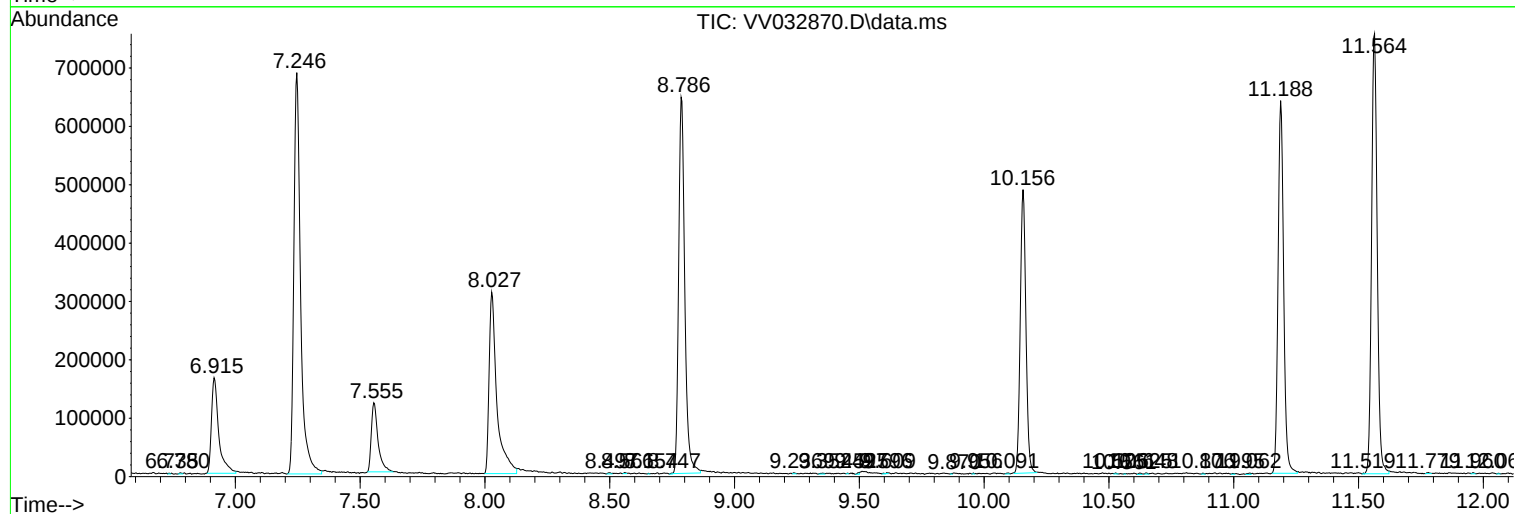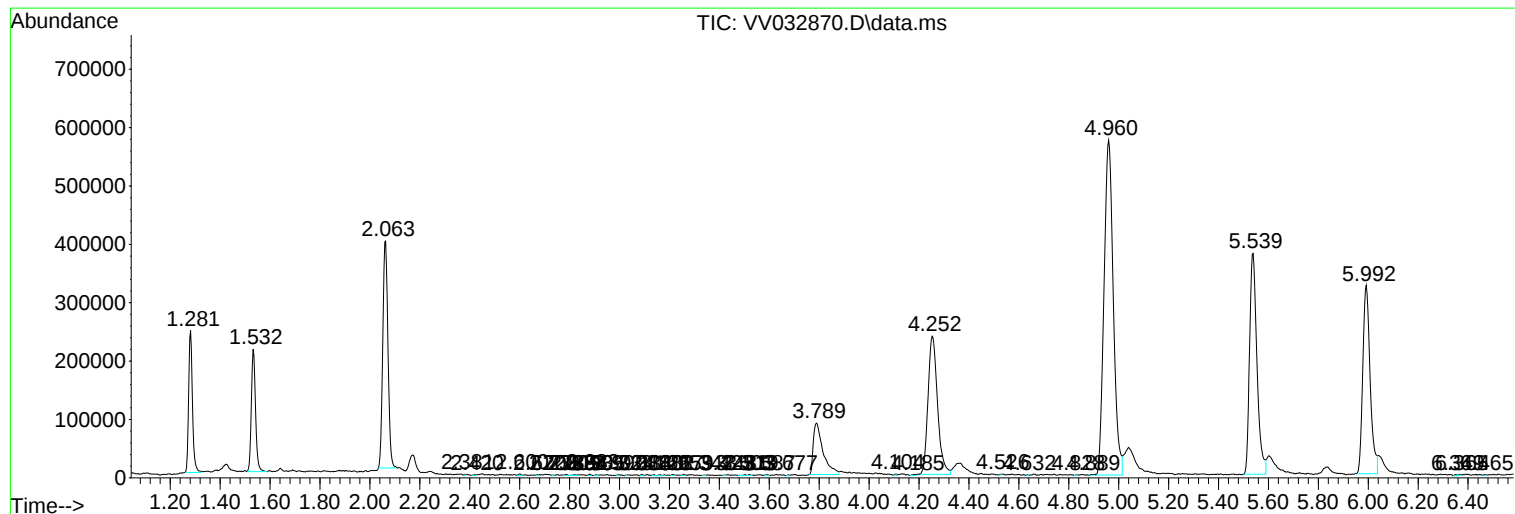

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032870.D
Acq On : 07 Nov 2023 15:28
Operator : SY/MD
Sample : 05226-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032870.D
Acq On : 07 Nov 2023 15:28
Operator : SY/MD
Sample : 05226-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------