

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032871.D
 Acq On : 07 Nov 2023 15:51
 Operator : SY/MD
 Sample : 05226-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rBV	237694	254847	17.25%	2.226%
2	1.532	146	153	166	rBV	205861	244139	16.53%	2.132%
3	2.063	309	318	329	rBV	390360	563530	38.14%	4.922%
4	2.513	455	458	460	rBV4	1046	699	0.05%	0.006%
5	2.542	464	467	468	rBV3	1468	921	0.06%	0.008%
6	2.606	485	487	490	rVB4	1705	802	0.05%	0.007%
7	2.728	523	525	529	rBV5	2245	1476	0.10%	0.013%
8	2.812	546	551	556	rBV7	1893	1809	0.12%	0.016%
9	2.838	556	559	562	rBV5	1442	1227	0.08%	0.011%
10	2.941	588	591	593	rBV4	1099	770	0.05%	0.007%
11	2.976	599	602	603	rBV3	1019	681	0.05%	0.006%
12	3.043	618	623	626	rBV7	1839	2158	0.15%	0.019%
13	3.111	642	644	646	rVB2	1598	615	0.04%	0.005%
14	3.124	646	648	651	rBV4	1206	811	0.05%	0.007%
15	3.143	651	654	657	rVB4	1274	786	0.05%	0.007%
16	3.175	662	664	668	rVB3	1522	863	0.06%	0.008%
17	3.204	668	673	674	rBV6	1373	990	0.07%	0.009%
18	3.281	694	697	700	rBV4	1039	857	0.06%	0.007%
19	3.307	703	705	706	rBV2	1482	681	0.05%	0.006%
20	3.371	720	725	726	rBV5	794	600	0.04%	0.005%
21	3.407	734	736	741	rVB7	1094	967	0.07%	0.008%
22	3.468	751	755	756	rBV4	1410	964	0.07%	0.008%
23	3.497	761	764	767	rBV5	1370	1051	0.07%	0.009%
24	3.516	768	770	773	rVB3	1905	949	0.06%	0.008%
25	3.551	778	781	783	rBV4	1260	738	0.05%	0.006%
26	3.616	798	801	802	rBV3	1197	723	0.05%	0.006%
27	3.635	805	807	810	rVB3	1828	1052	0.07%	0.009%
28	3.667	810	817	819	rBV6	1919	1575	0.11%	0.014%
29	3.680	819	821	825	rVB5	2051	1044	0.07%	0.009%
30	3.699	825	827	832	rBV5	1928	1190	0.08%	0.010%
31	3.748	840	842	846	rVB4	1576	1183	0.08%	0.010%
32	3.789	846	855	888	rBV2	91325	264353	17.89%	2.309%
33	4.130	959	961	963	rBV4	1901	1010	0.07%	0.009%
34	4.172	972	974	976	rBV3	980	598	0.04%	0.005%
35	4.256	986	1000	1020	rBV	237272	605014	40.95%	5.285%
36	4.728	1143	1147	1148	rBV4	1780	1017	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032871.D
 Acq On : 07 Nov 2023 15:51
 Operator : SY/MD
 Sample : 05226-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.873	1188	1192	1197	rBV8	1349	1348	0.09%	0.012%
38	4.960	1203	1219	1236	rBV2	561210	1477384	100.00%	12.905%
39	5.391	1350	1353	1356	rBV4	1797	1403	0.09%	0.012%
40	5.538	1388	1399	1414	rBV	372037	756472	51.20%	6.608%
41	5.992	1528	1540	1575	rBV	323122	720018	48.74%	6.289%
42	6.333	1642	1646	1649	rBV5	1540	1436	0.10%	0.013%
43	6.374	1658	1659	1661	rBV2	1761	986	0.07%	0.009%
44	6.429	1673	1676	1680	rBV6	1391	1201	0.08%	0.010%
45	6.455	1680	1684	1685	rVB4	1540	904	0.06%	0.008%
46	6.915	1817	1827	1863	rBV	161598	337683	22.86%	2.950%
47	7.246	1919	1930	1961	rBV	675087	1251617	84.72%	10.933%
48	7.554	2018	2026	2049	rBV	120104	224984	15.23%	1.965%
49	7.796	2098	2101	2104	rBV5	1826	1268	0.09%	0.011%
50	7.812	2104	2106	2108	rBV3	1453	626	0.04%	0.005%
51	7.892	2129	2131	2133	rBV3	1341	712	0.05%	0.006%
52	8.027	2164	2173	2208	rBV2	317774	677188	45.84%	5.915%
53	8.786	2399	2409	2440	rBV	625517	1082847	73.29%	9.458%
54	9.159	2523	2525	2528	rVB4	1926	761	0.05%	0.007%
55	9.175	2528	2530	2532	rBV3	1632	1041	0.07%	0.009%
56	9.326	2575	2577	2580	rVB4	2353	936	0.06%	0.008%
57	9.390	2593	2597	2599	rBV4	1487	1424	0.10%	0.012%
58	9.493	2624	2629	2631	rBV5	1410	1243	0.08%	0.011%
59	9.580	2654	2656	2657	rBV2	1513	584	0.04%	0.005%
60	9.641	2673	2675	2679	rBV3	1647	1129	0.08%	0.010%
61	9.741	2704	2706	2708	rBV3	1552	796	0.05%	0.007%
62	9.779	2716	2718	2721	rBV4	1531	937	0.06%	0.008%
63	9.837	2732	2736	2741	rBV7	1758	1948	0.13%	0.017%
64	9.921	2759	2762	2765	rBV5	1007	565	0.04%	0.005%
65	10.050	2799	2802	2804	rBV3	1090	752	0.05%	0.007%
66	10.156	2823	2835	2853	rBV	481797	774215	52.40%	6.763%
67	10.847	3046	3050	3052	rBV4	1392	971	0.07%	0.008%
68	10.879	3058	3060	3063	rBV4	1764	1043	0.07%	0.009%
69	10.998	3095	3097	3101	rBV4	1408	999	0.07%	0.009%
70	11.017	3101	3103	3106	rVB4	2364	1315	0.09%	0.011%
71	11.062	3113	3117	3119	rBV4	1494	1197	0.08%	0.010%
72	11.082	3119	3123	3126	rVB6	1082	775	0.05%	0.007%
73	11.111	3126	3132	3134	rBV8	2111	1593	0.11%	0.014%
74	11.188	3146	3156	3175	rBV	627856	967006	65.45%	8.447%
75	11.345	3202	3205	3208	rBV5	2389	1677	0.11%	0.015%
76	11.416	3224	3227	3228	rBV3	1334	796	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032871.D
 Acq On : 07 Nov 2023 15:51
 Operator : SY/MD
 Sample : 05226-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.484	3244	3248	3251	rBV6	1736	1809	0.12%	0.016%
78	11.564	3261	3273	3295	rBV	739599	1157462	78.35%	10.110%
79	11.902	3374	3378	3381	rBV6	1620	1338	0.09%	0.012%
80	11.943	3389	3391	3393	rBV3	1211	699	0.05%	0.006%
81	12.078	3429	3433	3436	rBV6	2144	2192	0.15%	0.019%
82	12.201	3467	3471	3474	rBV5	1916	1544	0.10%	0.013%
83	12.284	3495	3497	3499	rBV3	1461	816	0.06%	0.007%
84	12.332	3509	3512	3517	rVB7	2390	1693	0.11%	0.015%
85	12.355	3517	3519	3522	rBV4	2283	1585	0.11%	0.014%
86	12.467	3552	3554	3556	rVB3	1547	791	0.05%	0.007%
87	12.509	3565	3567	3569	rBV3	1515	764	0.05%	0.007%
88	12.631	3603	3605	3606	rBV2	1136	567	0.04%	0.005%
89	12.802	3657	3658	3660	rBV2	1477	649	0.04%	0.006%
90	12.853	3671	3674	3677	rBV4	1150	960	0.06%	0.008%
91	13.156	3765	3768	3769	rBV3	1421	792	0.05%	0.007%
92	13.201	3779	3782	3784	rBV3	1261	924	0.06%	0.008%
93	13.258	3797	3800	3804	rBV6	1323	1193	0.08%	0.010%
94	13.406	3838	3846	3848	rBV9	2321	2776	0.19%	0.024%
95	13.538	3884	3887	3889	rBV4	1291	854	0.06%	0.007%
96	13.828	3975	3977	3983	rBV7	1961	1822	0.12%	0.016%
97	13.889	3994	3996	4000	rBV5	783	681	0.05%	0.006%
98	14.075	4052	4054	4055	rBV2	1521	516	0.03%	0.005%
99	14.104	4061	4063	4065	rBV3	1475	743	0.05%	0.006%
100	14.467	4174	4176	4181	rBV5	1070	931	0.06%	0.008%




Sum of corrected areas: 11448571

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032871.D
Acq On : 07 Nov 2023 15:51
Operator : SY/MD
Sample : 05226-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

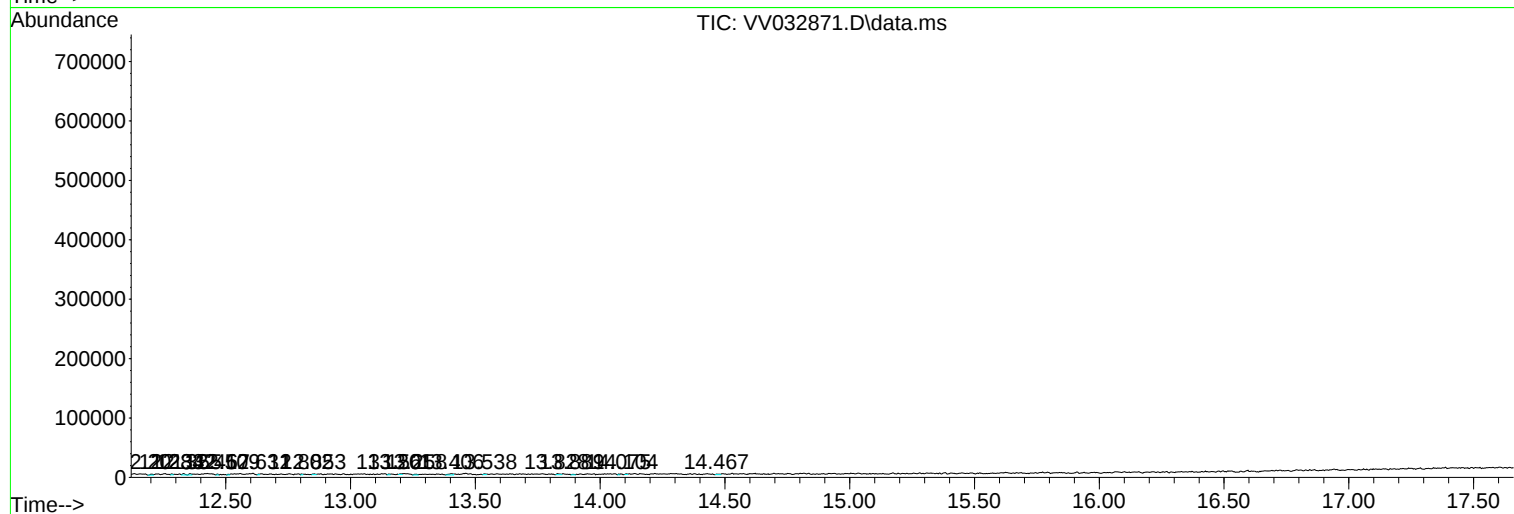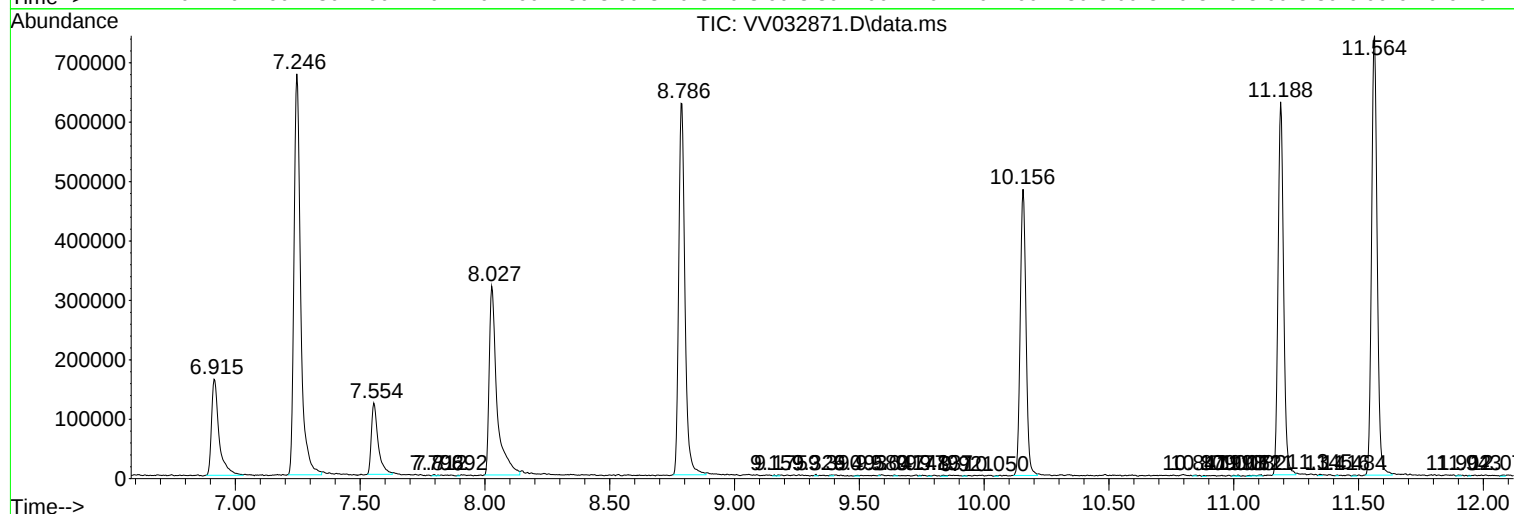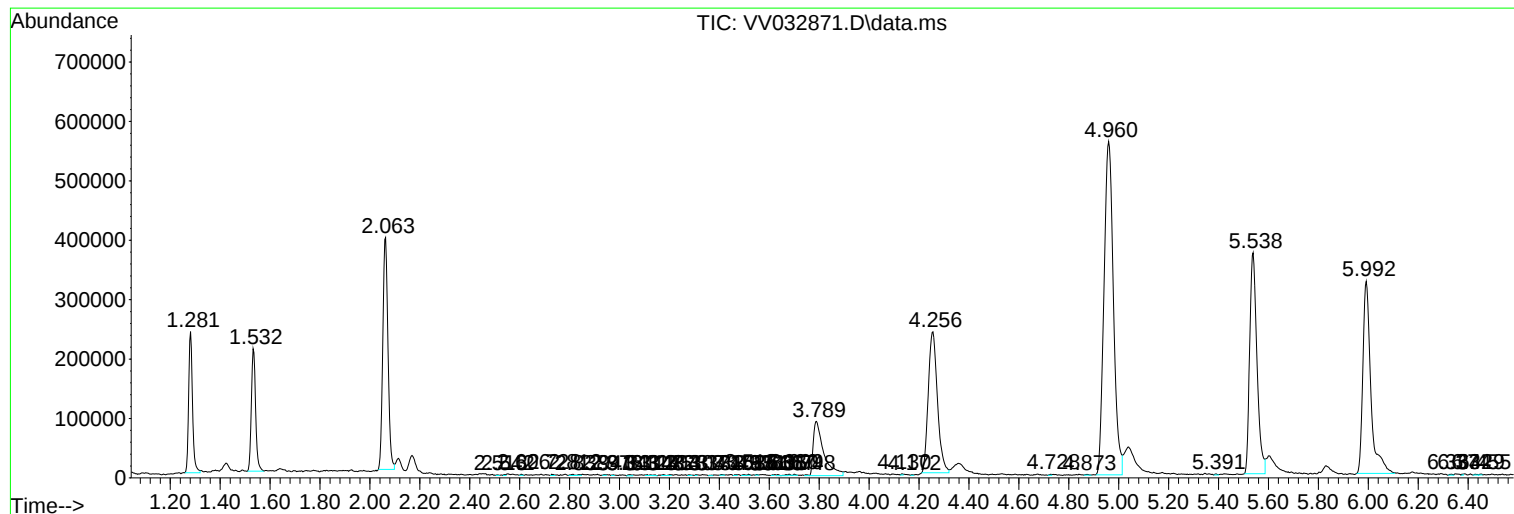

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032871.D
Acq On : 07 Nov 2023 15:51
Operator : SY/MD
Sample : 05226-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032871.D
Acq On : 07 Nov 2023 15:51
Operator : SY/MD
Sample : 05226-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc