

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032872.D
 Acq On : 07 Nov 2023 16:14
 Operator : SY/MD
 Sample : 05226-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

Signal : TIC: VV032872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	152025	158143	13.71%	1.611%
2	1.532	147	153	170	rVB	147894	175939	15.25%	1.793%
3	2.063	310	318	333	rVB	273345	393646	34.12%	4.011%
4	2.445	434	437	439	rBV4	2244	1480	0.13%	0.015%
5	2.641	496	498	502	rBV5	1035	801	0.07%	0.008%
6	2.738	524	528	533	rBV7	1317	1602	0.14%	0.016%
7	2.821	552	554	555	rBV2	893	417	0.04%	0.004%
8	2.899	574	578	579	rBV4	1802	1146	0.10%	0.012%
9	2.934	586	589	591	rBV4	1805	1229	0.11%	0.013%
10	2.995	604	608	611	rBV6	1807	1377	0.12%	0.014%
11	3.024	615	617	618	rBV2	1633	736	0.06%	0.007%
12	3.069	625	631	632	rBV6	1797	1694	0.15%	0.017%
13	3.182	663	666	667	rBV3	1196	531	0.05%	0.005%
14	3.214	673	676	682	rBV9	1597	1516	0.13%	0.015%
15	3.358	719	721	724	rBV4	1283	878	0.08%	0.009%
16	3.416	736	739	740	rBV3	1091	480	0.04%	0.005%
17	3.539	775	777	779	rBV3	1191	611	0.05%	0.006%
18	3.567	783	786	789	rBV5	986	1001	0.09%	0.010%
19	3.593	792	794	795	rBV2	994	464	0.04%	0.005%
20	3.641	806	809	810	rBV2	1310	629	0.05%	0.006%
21	3.674	817	819	821	rBV3	1206	688	0.06%	0.007%
22	3.789	844	855	879	rBV	82171	224619	19.47%	2.289%
23	4.256	986	1000	1020	rBV	195187	492138	42.65%	5.014%
24	4.667	1125	1128	1129	rBV3	958	432	0.04%	0.004%
25	4.699	1135	1138	1139	rBV3	1413	739	0.06%	0.008%
26	4.783	1160	1164	1166	rBV5	1279	1114	0.10%	0.011%
27	4.812	1171	1173	1176	rVV4	1190	789	0.07%	0.008%
28	4.844	1180	1183	1184	rBV3	848	417	0.04%	0.004%
29	4.960	1203	1219	1237	rBV2	434856	1153784	100.00%	11.755%
30	5.262	1311	1313	1318	rVB5	2531	2011	0.17%	0.020%
31	5.284	1318	1320	1323	rBV3	1562	947	0.08%	0.010%
32	5.400	1354	1356	1358	rBV3	1529	647	0.06%	0.007%
33	5.461	1373	1375	1378	rBV4	1653	1026	0.09%	0.010%
34	5.538	1387	1399	1415	rBV	375178	772664	66.97%	7.872%
35	5.992	1528	1540	1577	rBV	259566	594970	51.57%	6.062%
36	6.497	1693	1697	1699	rBV5	1686	1142	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032872.D
 Acq On : 07 Nov 2023 16:14
 Operator : SY/MD
 Sample : 05226-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.567	1716	1719	1720	rBV3	1622	958	0.08%	0.010%
38	6.715	1764	1765	1766	rBV	1595	607	0.05%	0.006%
39	6.757	1773	1778	1780	rBV8	1969	1736	0.15%	0.018%
40	6.786	1784	1787	1789	rVB4	1456	1001	0.09%	0.010%
41	6.821	1794	1798	1799	rBV4	1244	878	0.08%	0.009%
42	6.915	1816	1827	1850	rBV	128959	268862	23.30%	2.739%
43	7.246	1919	1930	1958	rBV	496377	936372	81.16%	9.540%
44	7.558	2018	2027	2056	rVB	93414	183483	15.90%	1.869%
45	7.812	2104	2106	2107	rBV2	1238	502	0.04%	0.005%
46	7.947	2147	2148	2150	rBV	1144	637	0.06%	0.006%
47	7.982	2157	2159	2161	rBV3	1275	437	0.04%	0.004%
48	8.027	2164	2173	2204	rBV	272622	590220	51.16%	6.013%
49	8.480	2312	2314	2318	rBV5	1264	1033	0.09%	0.011%
50	8.580	2344	2345	2349	rBV4	2093	1623	0.14%	0.017%
51	8.789	2397	2410	2431	rBV	641497	1099787	95.32%	11.205%
52	9.117	2509	2512	2515	rBV4	1748	1297	0.11%	0.013%
53	9.339	2579	2581	2585	rBV5	1314	601	0.05%	0.006%
54	9.439	2611	2612	2617	rBV4	943	708	0.06%	0.007%
55	9.487	2624	2627	2628	rBV3	1239	759	0.07%	0.008%
56	9.554	2645	2648	2650	rBV4	1702	1154	0.10%	0.012%
57	9.677	2684	2686	2688	rBV3	1355	655	0.06%	0.007%
58	9.786	2717	2720	2724	rBV5	1511	1497	0.13%	0.015%
59	9.818	2728	2730	2731	rBV2	950	539	0.05%	0.005%
60	9.902	2755	2756	2760	rBV4	1290	828	0.07%	0.008%
61	10.056	2802	2804	2809	rBV6	1968	1480	0.13%	0.015%
62	10.085	2809	2813	2816	rBV5	2046	1386	0.12%	0.014%
63	10.156	2822	2835	2854	rBV	441457	710352	61.57%	7.237%
64	10.487	2936	2938	2939	rBV2	1291	526	0.05%	0.005%
65	10.673	2994	2996	3000	rVB5	1314	473	0.04%	0.005%
66	10.705	3003	3006	3009	rBV5	1713	1235	0.11%	0.013%
67	10.776	3023	3028	3031	rBV6	2020	2134	0.18%	0.022%
68	10.795	3032	3034	3039	rVB6	1787	1431	0.12%	0.015%
69	10.860	3051	3054	3057	rBV3	1116	866	0.08%	0.009%
70	10.918	3069	3072	3075	rVB5	1997	1183	0.10%	0.012%
71	10.934	3075	3077	3079	rBV3	2301	1268	0.11%	0.013%
72	10.998	3095	3097	3100	rBV4	2148	1425	0.12%	0.015%
73	11.130	3136	3138	3140	rBV3	1513	658	0.06%	0.007%
74	11.188	3143	3156	3183	rBV	643992	1009256	87.47%	10.283%
75	11.487	3246	3249	3250	rBV3	1125	582	0.05%	0.006%
76	11.564	3262	3273	3292	rBV	610156	970912	84.15%	9.892%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
 Data File : VV032872.D
 Acq On : 07 Nov 2023 16:14
 Operator : SY/MD
 Sample : 05226-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.802	3345	3347	3349	rBV3	1297	732	0.06%	0.007%
78	11.950	3391	3393	3396	rBV4	2201	1121	0.10%	0.011%
79	12.213	3474	3475	3478	rVB3	1338	535	0.05%	0.005%
80	12.316	3504	3507	3509	rBV4	1171	747	0.06%	0.008%
81	12.422	3537	3540	3542	rBV3	1430	890	0.08%	0.009%
82	12.490	3559	3561	3565	rBV5	1289	760	0.07%	0.008%
83	12.554	3579	3581	3584	rBV4	1158	653	0.06%	0.007%
84	12.586	3589	3591	3594	rVB4	1958	836	0.07%	0.009%
85	12.602	3594	3596	3599	rBV3	1262	949	0.08%	0.010%
86	12.692	3622	3624	3626	rBV3	1441	618	0.05%	0.006%
87	12.734	3635	3637	3640	rBV4	901	539	0.05%	0.005%
88	12.750	3640	3642	3644	rBV3	1497	912	0.08%	0.009%
89	12.831	3663	3667	3669	rBV5	1790	1460	0.13%	0.015%
90	12.946	3700	3703	3705	rBV5	1429	815	0.07%	0.008%
91	12.985	3713	3715	3717	rBV2	1154	811	0.07%	0.008%
92	13.040	3729	3732	3733	rBV3	1481	863	0.07%	0.009%
93	13.072	3740	3742	3744	rBV4	1258	606	0.05%	0.006%
94	13.303	3812	3814	3818	rBV5	1683	1149	0.10%	0.012%
95	13.326	3818	3821	3824	rBV4	893	638	0.06%	0.007%
96	13.487	3868	3871	3872	rBV4	1364	790	0.07%	0.008%
97	13.898	3994	3999	4000	rBV5	1667	1415	0.12%	0.014%
98	14.120	4066	4068	4071	rBV3	1006	590	0.05%	0.006%
99	14.519	4189	4192	4194	rBV4	1309	743	0.06%	0.008%
100	14.770	4265	4270	4273	rBV6	2375	2110	0.18%	0.021%




Sum of corrected areas: 9815070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032872.D
Acq On : 07 Nov 2023 16:14
Operator : SY/MD
Sample : 05226-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

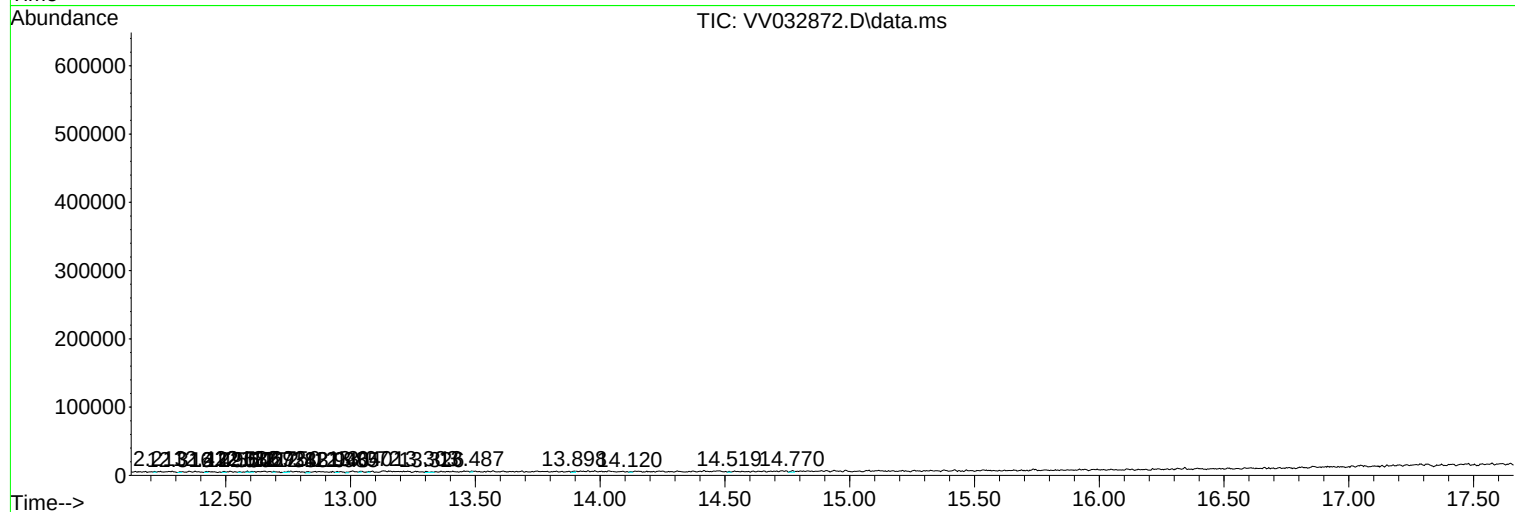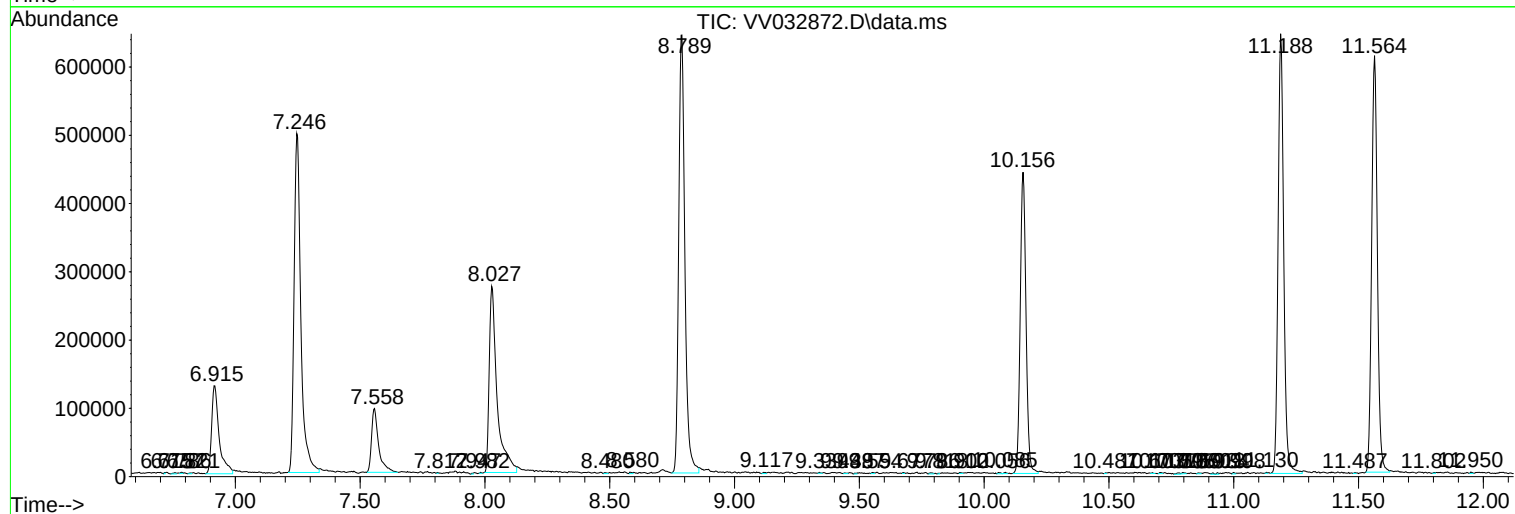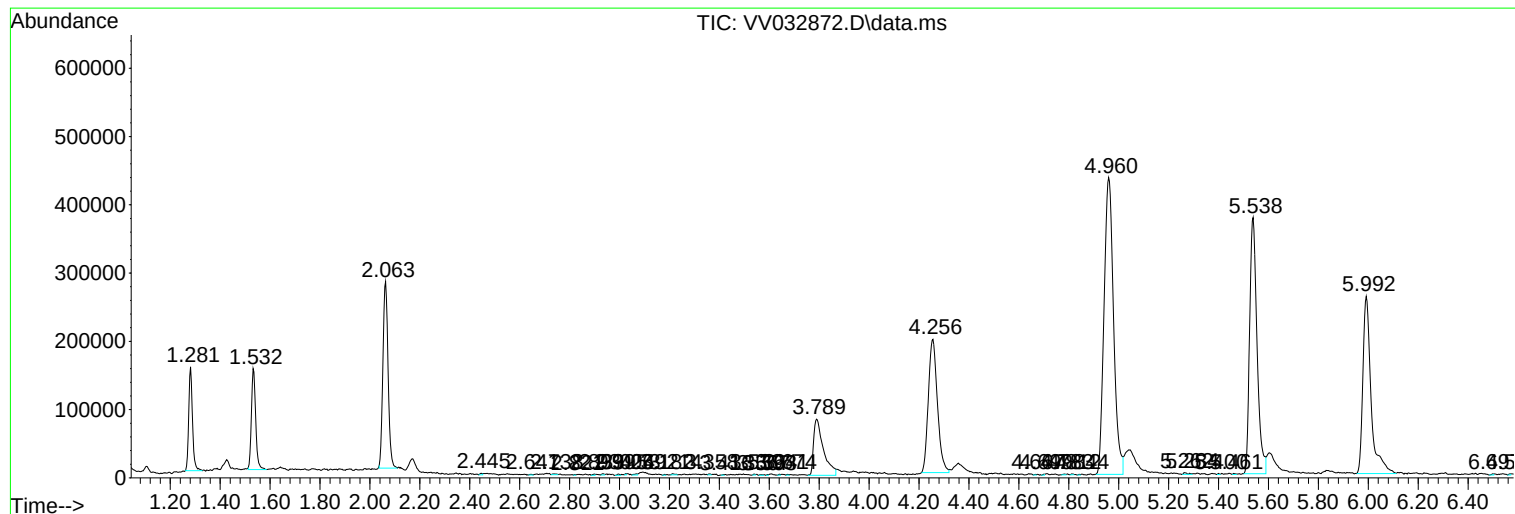

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032872.D
Acq On : 07 Nov 2023 16:14
Operator : SY/MD
Sample : 05226-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110723\
Data File : VV032872.D
Acq On : 07 Nov 2023 16:14
Operator : SY/MD
Sample : 05226-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------