

Data File : VV013543.D
Acq On : 08 Nov 2019 16:56
Operator : SY/MD
Sample : K5747-03MSD
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J00MSD

Quant Time: Nov 08 22:54:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	396408	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	391240	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	187326	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	88699	5.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.20%
7) Chloroethane-d5	1.58	69	81291	5.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.60%
11) 1,1-Dichloroethene-d2	2.13	63	151261	4.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.60%
20) 2-Butanone-d5	3.92	46	279180	46.61	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.22%
24) Chloroform-d	4.40	84	209652	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.08	65	117273	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.10	84	397674	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.12	67	140792	5.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.40%
41) Toluene-d8	7.36	98	314137	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.66	79	50109	4.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.40%
46) 2-Hexanone-d5	8.13	63	183891	44.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	96681	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	173224	5.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.00%

Target Compounds

					Qvalue
12) 1,1-Dichloroethene	2.14	96	87469	3.669 ug/L	95
13) Acetone	2.18	43	27995	7.705 ug/L	96
15) Methyl Acetate	2.30	43	8504	0.783 ug/L #	55
25) Chloroform	4.42	83	24549	0.408 ug/L	99
33) Benzene	5.14	78	489769	4.029 ug/L	100
34) Trichloroethene	5.96	95	124436	3.796 ug/L	98
35) Methylcyclohexane	6.12	83	33728	0.677 ug/L #	19
42) Toluene	7.43	91	510671	4.039 ug/L	100
48) 2-Hexanone	8.18	43	14221	1.168 ug/L #	87
51) Chlorobenzene	8.92	112	372998	4.472 ug/L	99
52) Ethylbenzene	9.05	91	8299	0.061 ug/L	98
53) m,p-xylene	9.18	106	8074	0.160 ug/L	90
54) o-xylene	9.59	106	4821	0.099 ug/L	84
67) 1,3,5-Trichlorobenzene	12.69	180	2892	0.059 ug/L #	28
68) 1,2,4-trichlorobenzene	13.31	180	4070	0.104 ug/L	94
69) Naphthalene	13.55	128	980744	18.589 ug/L	100
70) 1,2,3-Trichlorobenzene	13.79	180	3101	0.085 ug/L	85

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110819\
Quantitation Report (Not Reviewed)

Data File : VV013543.D
Acq On : 08 Nov 2019 16:56
Operator : SY/MD
Sample : K5747-03MSD
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J00MSD

Quant Time: Nov 08 22:54:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV013543.D
Acq On : 08 Nov 2019 16:56
Operator : SY/MD
Sample : K5747-03MSD
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J00MSD

Quant Time: Nov 08 22:54:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

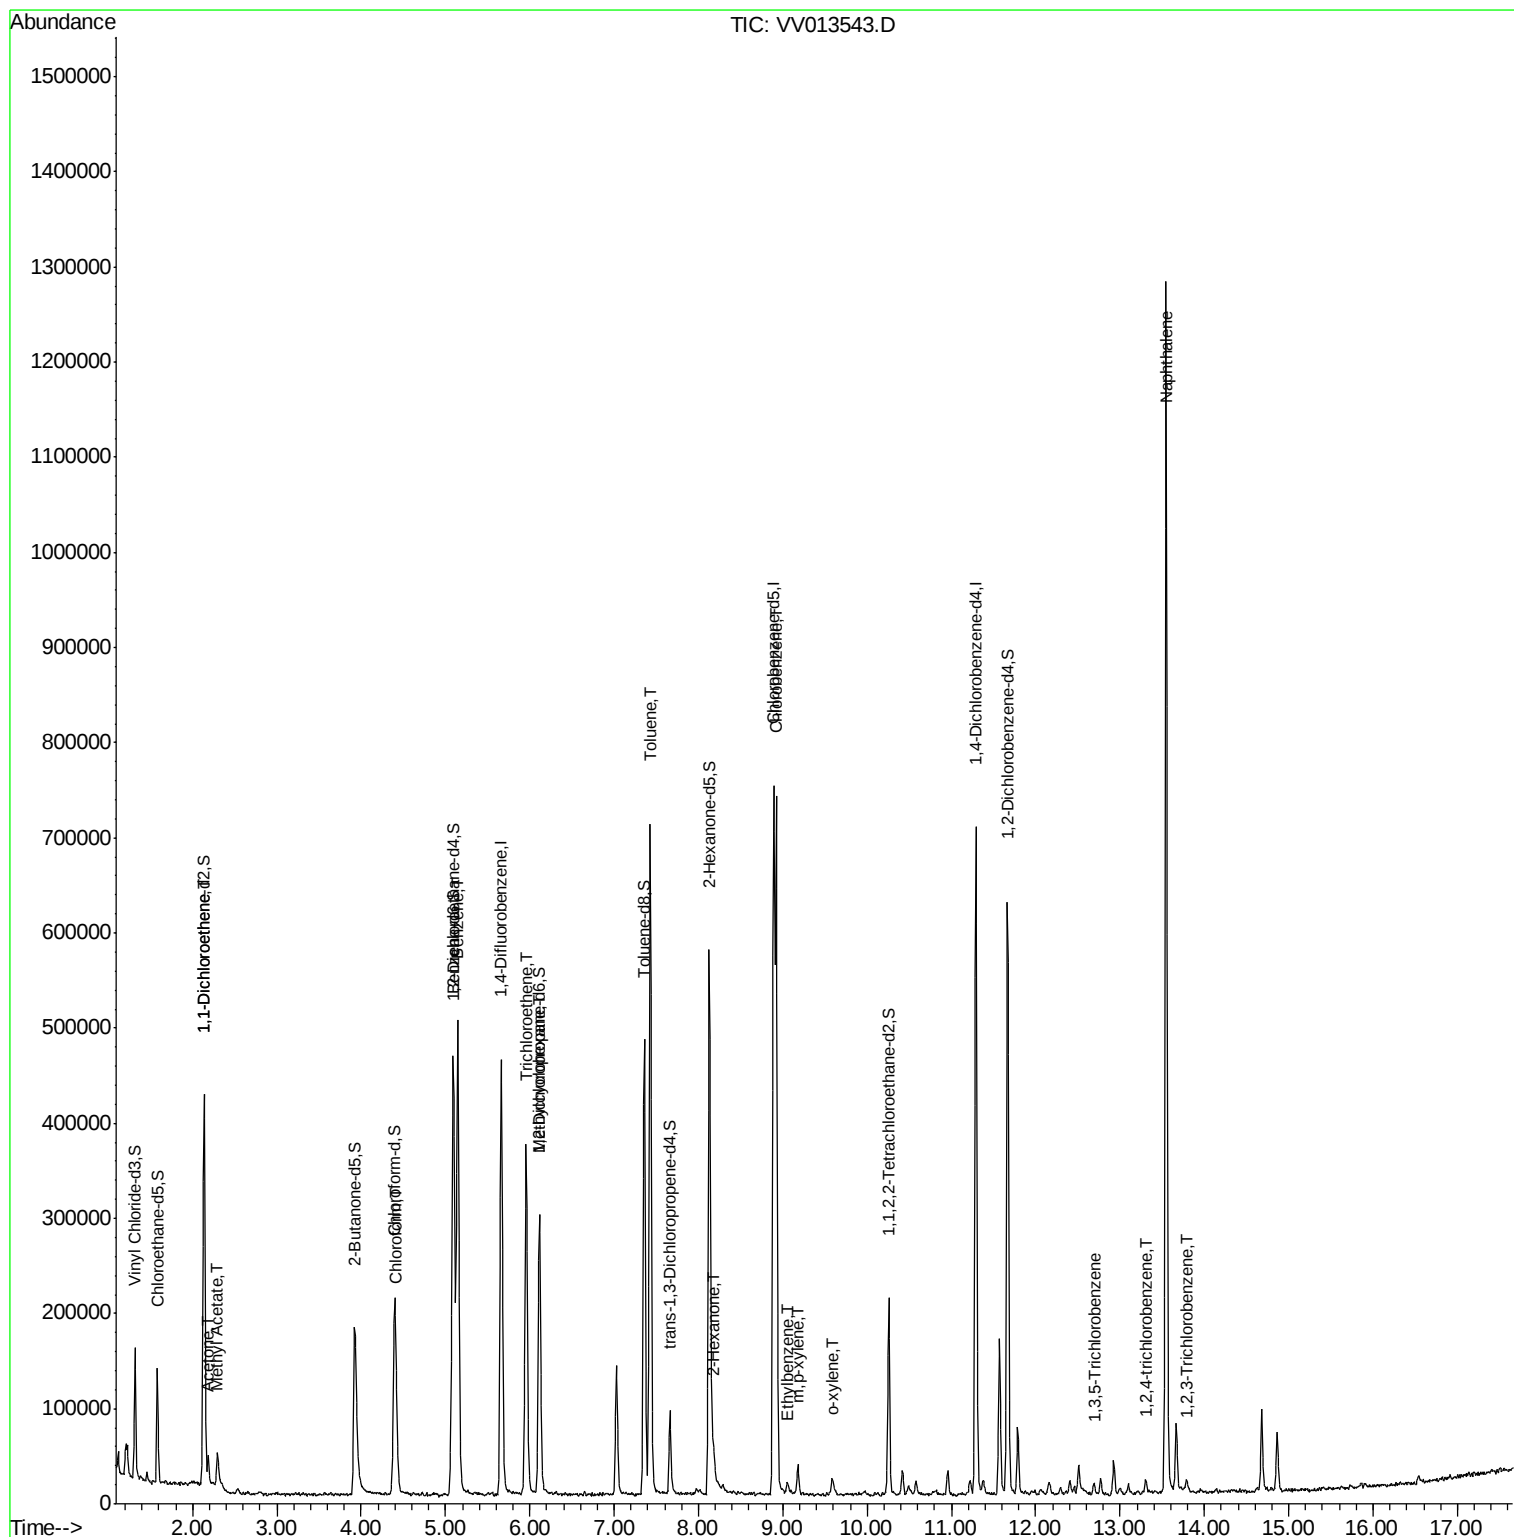

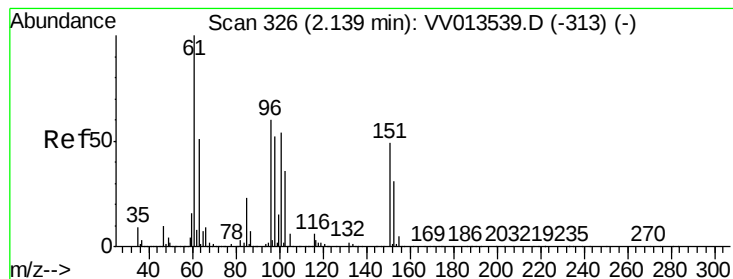

#12

1,1-Dichloroethene

Concen: 3.669 ug/L

RT: 2.14 min Scan# 327

Delta R.T. 0.00 min

Lab File: VV013543.D

Acq: 08 Nov 2019 16:56

Instrument :

MSVOA_V

ClientSampleId :

F2J00MSD





Tgt Ion: 96 Resp: 87469

Ion Ratio Lower Upper

96 100

61 160.6 117.1 217.5

63 103.4 68.5 127.1

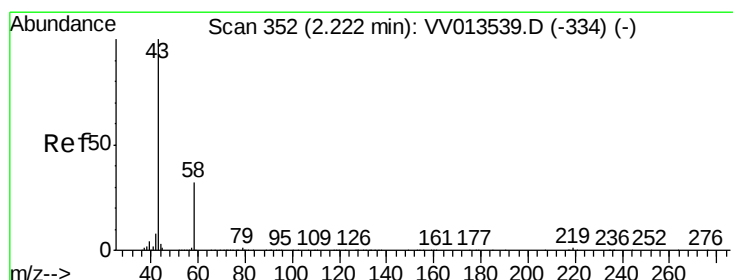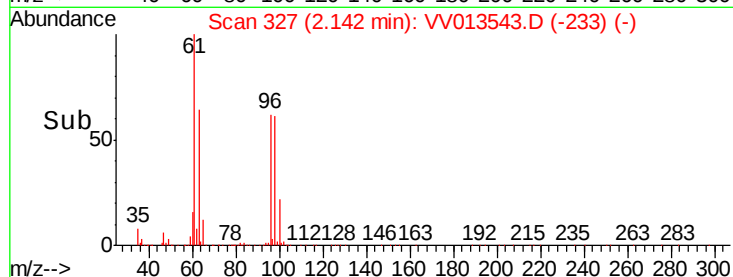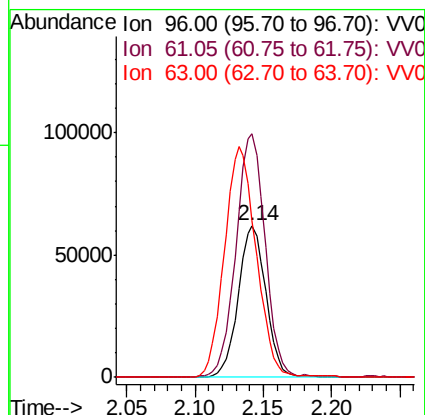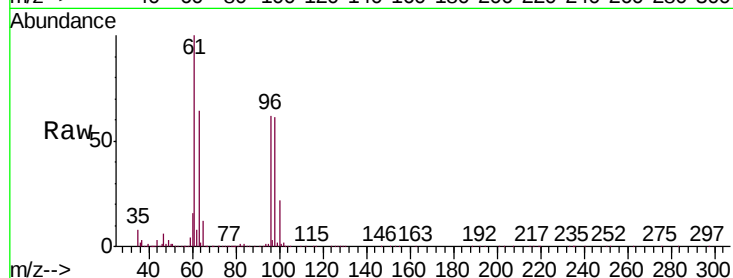

#13

Acetone

Concen: 7.705 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV013543.D




Acq: 08 Nov 2019 16:56


Tgt Ion: 43 Resp: 27995

Ion Ratio Lower Upper

43 100

58 28.3 0.0 60.8


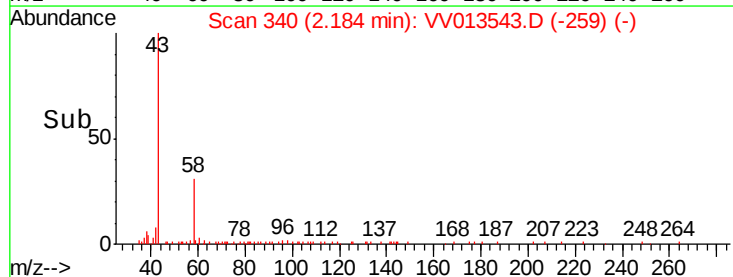
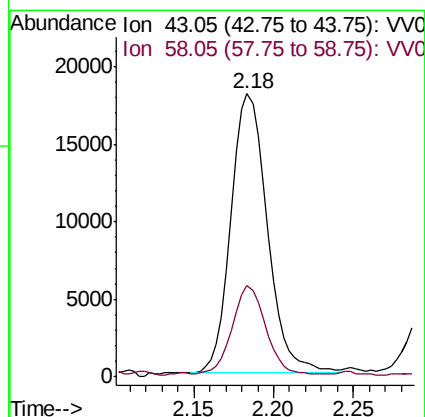
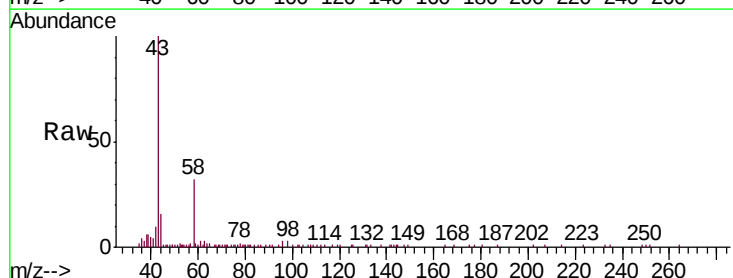


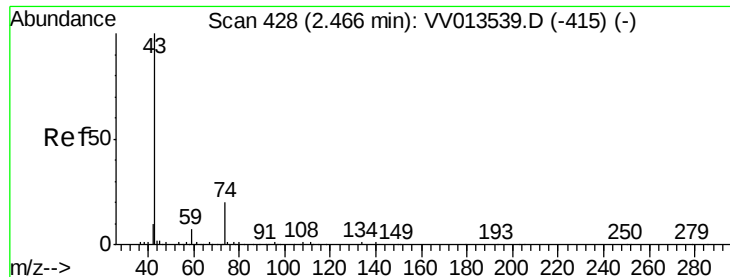

#15
Methyl Acetate
Concen: 0.783 ug/L
RT: 2.30 min Scan# 375
Delta R.T. -0.17 min
Lab File: VV013543.D
Acq: 08 Nov 2019 16:56




Instrument :
MSVOA_V
ClientSampleId :
F2J00MSD


Tgt Ion: 43 Resp: 8504
Ion Ratio Lower Upper
43 100
74 1.7 19.4 29.0#

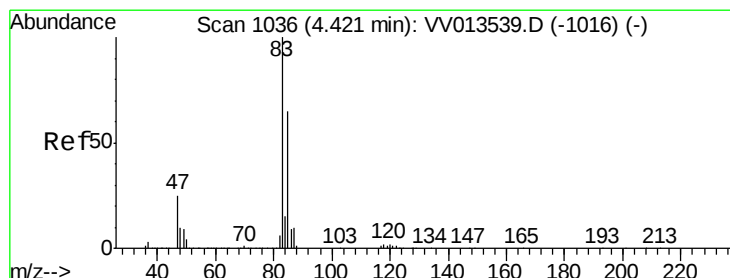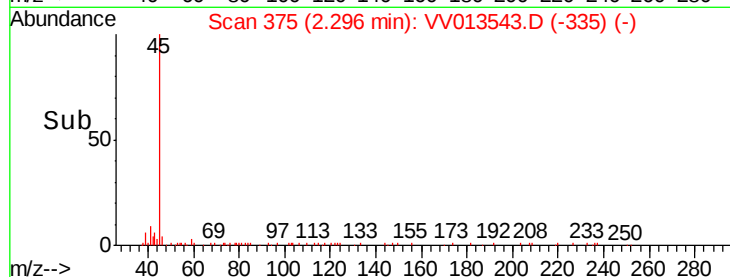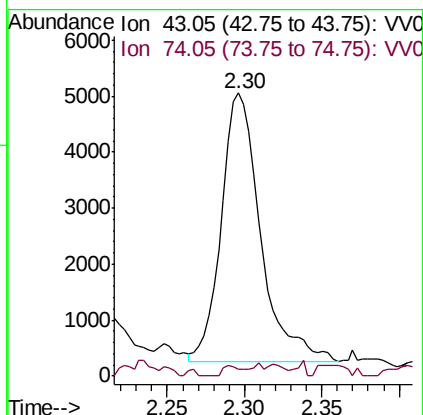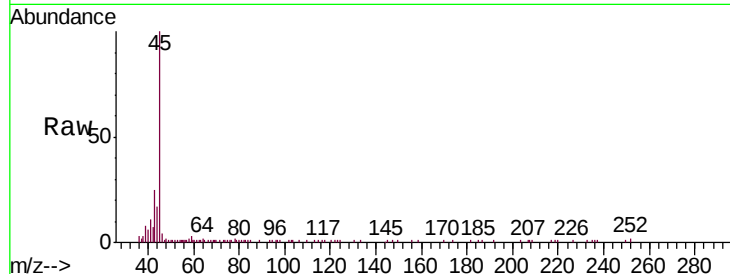

#25
Chloroform
Concen: 0.408 ug/L
RT: 4.42 min Scan# 1036
Delta R.T. 0.00 min
Lab File: VV013543.D
Acq: 08 Nov 2019 16:56

Tgt Ion: 83 Resp: 24549
Ion Ratio Lower Upper
83 100
85 65.4 46.3 86.1

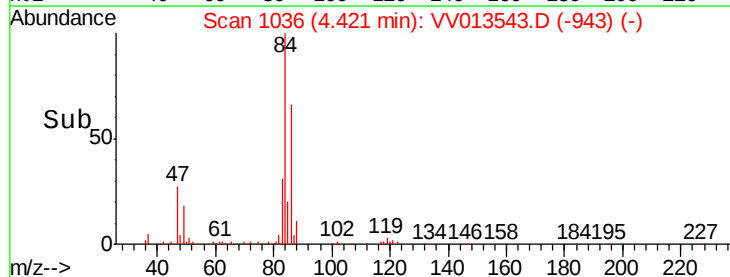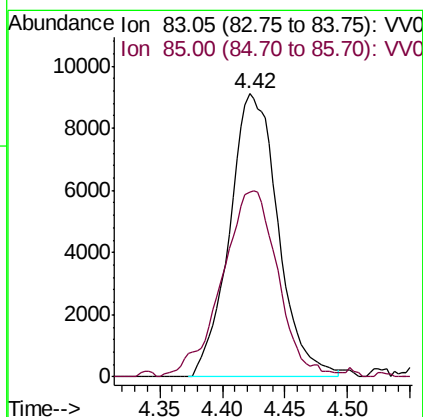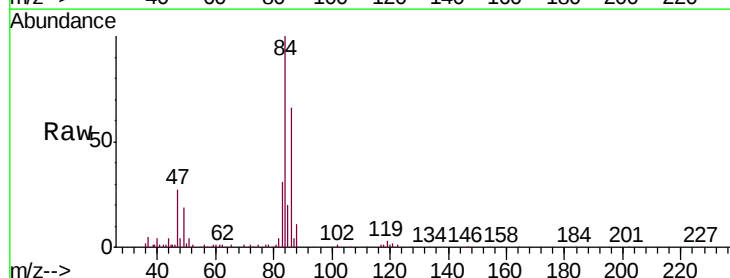

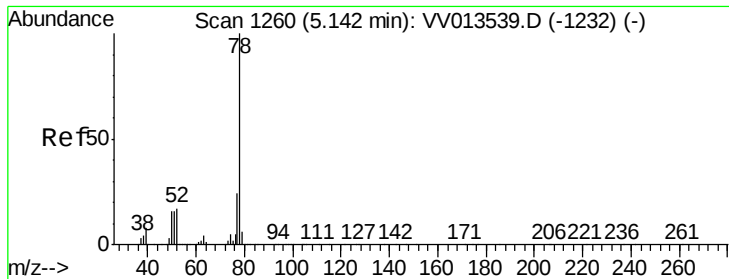

#33

Benzene

Concen: 4.029 ug/L

RT: 5.14 min Scan# 1261

Delta R.T. 0.00 min

Lab File: VV013543.D

Acq: 08 Nov 2019 16:56


Instrument :

MSVOA_V




ClientSampleId :

F2J00MSD

Tgt Ion: 78 Resp: 489769

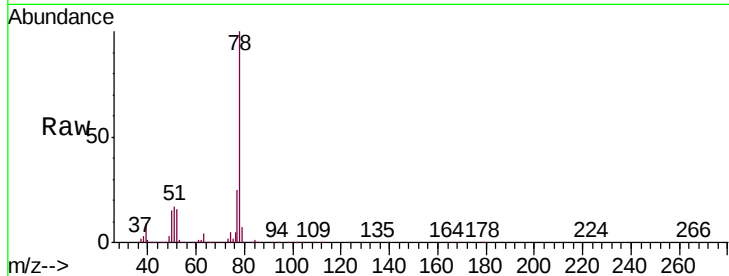

Abundance Ion 78.10 (77.80 to 78.80): VV0

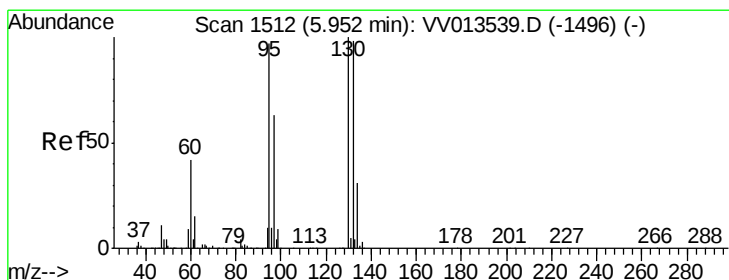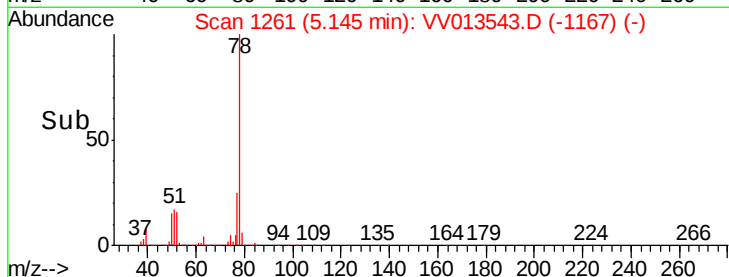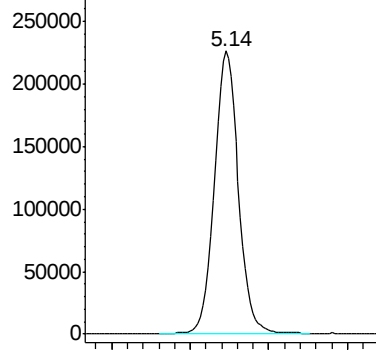

#34

Trichloroethene

Concen: 3.796 ug/L

RT: 5.96 min Scan# 1514

Delta R.T. 0.01 min

Lab File: VV013543.D

Acq: 08 Nov 2019 16:56

Tgt Ion: 95 Resp: 124436


Ion	Ratio	Lower	Upper
95	100		
97	63.0	44.7	83.1
132	103.5	71.6	133.0
130	111.2	74.6	138.6

95 100

97 63.0 44.7 83.1

132 103.5 71.6 133.0

130 111.2 74.6 138.6


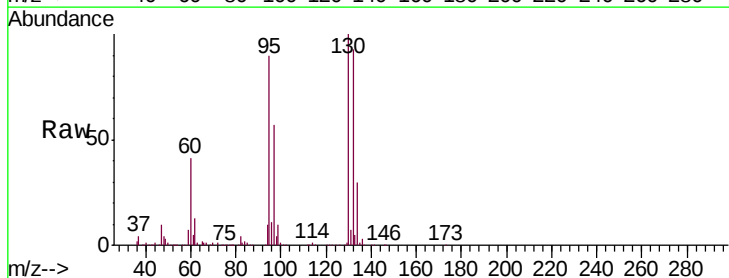



Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

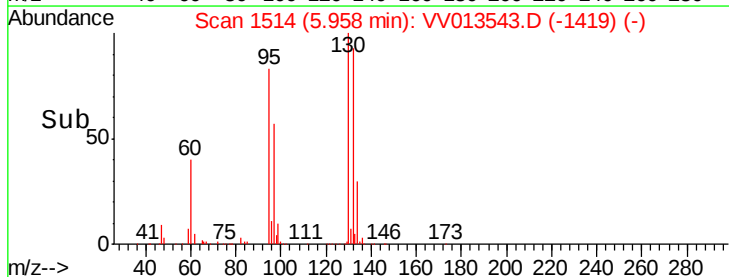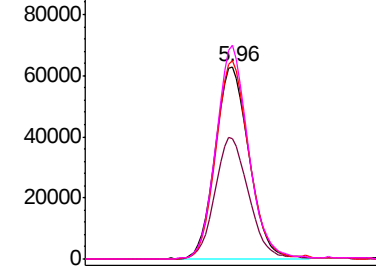

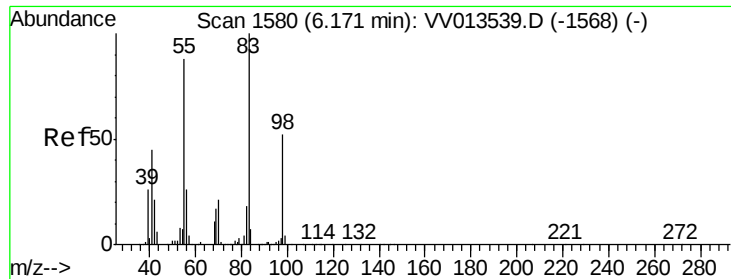

#35

Methylcyclohexane

Concen: 0.677 ug/L

RT: 6.12 min Scan# 1563

Delta R.T. -0.05 min

Lab File: VV013543.D

Acq: 08 Nov 2019 16:56

Instrument :

MSVOA_V

ClientSampleId :

F2J00MSD


Tgt Ion: 83 Resp: 33728

Ion Ratio Lower Upper

83 100

55 1.1 63.8 95.8#




98 2.7 38.4 57.6#

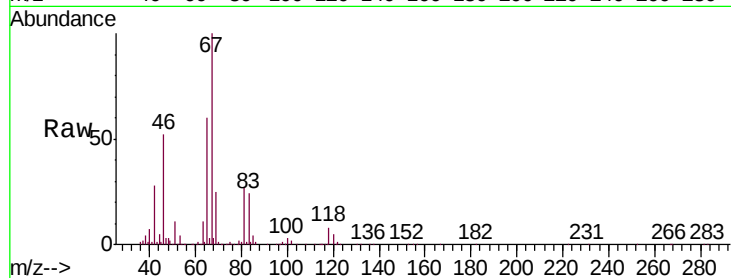

Abundance Ion 83.15 (82.85 to 83.85): VV0

Ion 55.10 (54.80 to 55.80): VV0

Ion 98.15 (97.85 to 98.85): VV0

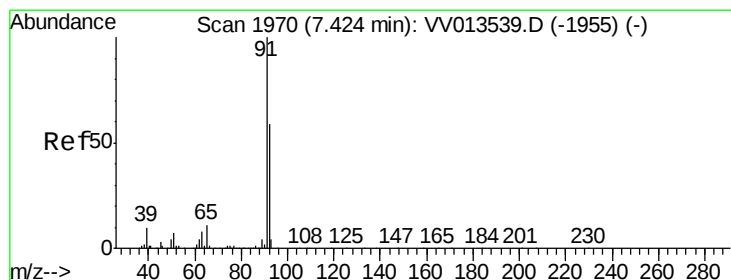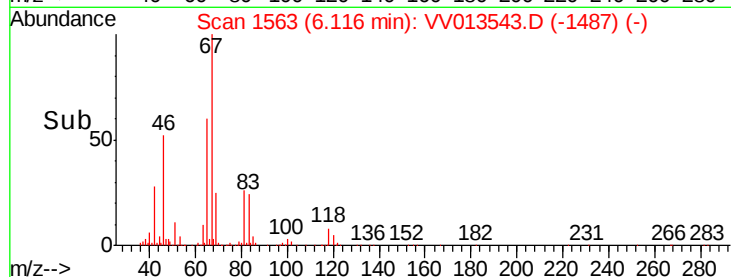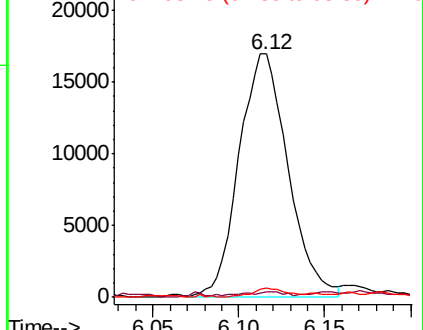

#42

Toluene

Concen: 4.039 ug/L

RT: 7.43 min Scan# 1971

Delta R.T. 0.00 min

Lab File: VV013543.D


Acq: 08 Nov 2019 16:56

Tgt Ion: 91 Resp: 510671

Ion Ratio Lower Upper



91 100


92 59.1 41.4 77.0

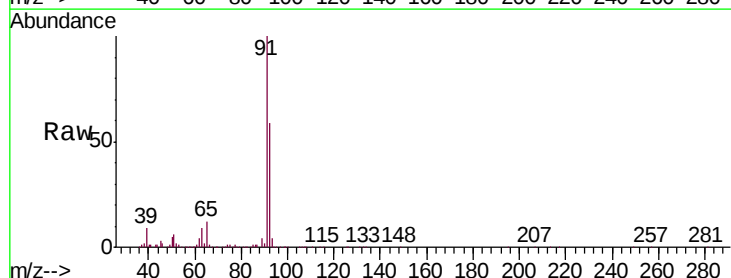

Abundance Ion 91.15 (90.85 to 91.85): VV0

Ion 92.15 (91.85 to 92.85): VV0

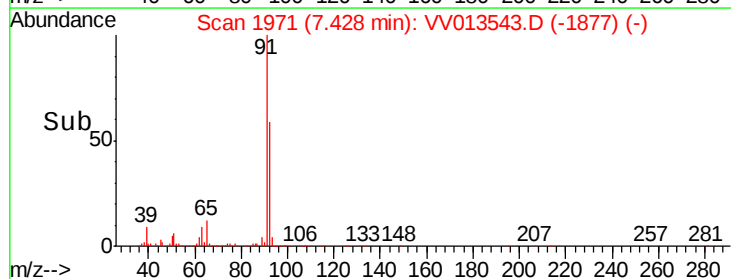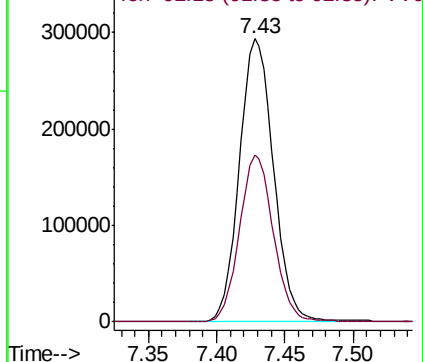


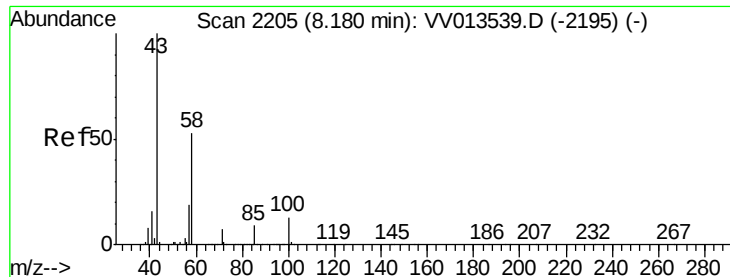

#48
2-Hexanone
Concen: 1.168 ug/L
RT: 8.18 min Scan# 2205
Delta R.T. 0.00 min
Lab File: VV013543.D
Acq: 08 Nov 2019 16:56

Instrument :
MSVOA_V
ClientSampleId :
F2J00MSD

Tgt Ion	Ratio	Lower	Upper
43	100		
58	51.2	43.8	65.8
57	0.0	15.0	22.6
100	11.6	9.8	14.6

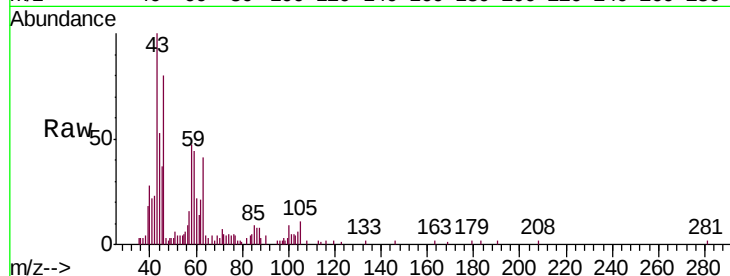




Abundance

Ion 43.05 (42.75 to 43.75): VV013543.D (-2195) (-)

Ion 58.05 (57.75 to 58.75): VV013543.D (-2195) (-)


Ion 57.20 (56.90 to 57.90): VV013543.D (-2195) (-)

Ion 100.15 (99.85 to 100.85): VV013543.D (-2195) (-)

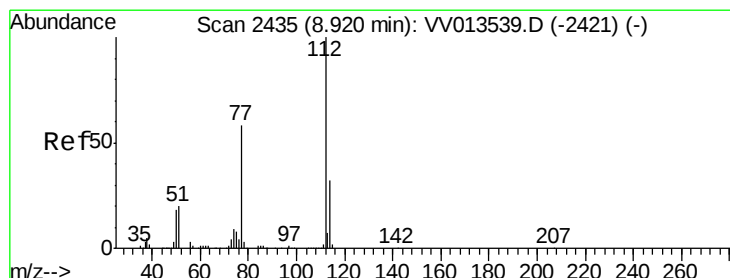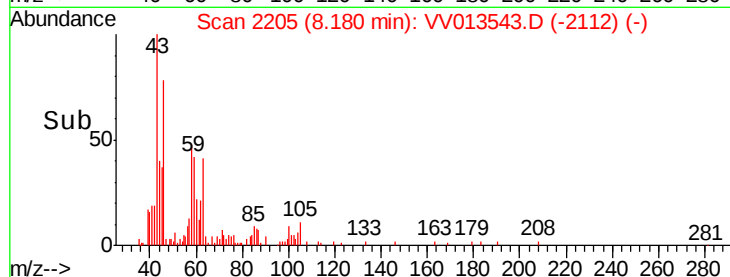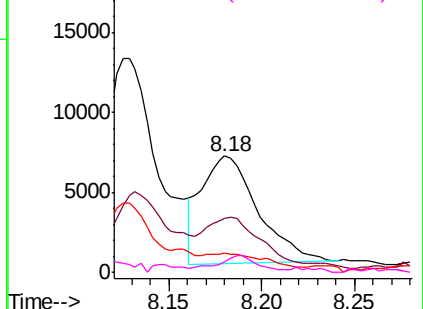

#51
Chlorobenzene
Concen: 4.472 ug/L
RT: 8.92 min Scan# 2436
Delta R.T. 0.00 min
Lab File: VV013543.D
Acq: 08 Nov 2019 16:56

Tgt Ion	Ratio	Lower	Upper
112	100		
114	31.5	22.6	42.0
77	58.2	46.2	69.2


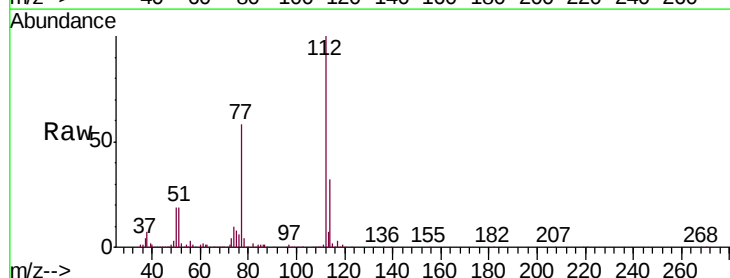



Abundance

Ion 112.10 (111.80 to 112.80): VV013543.D (-2432) (-)

Ion 114.05 (113.75 to 114.75): VV013543.D (-2432) (-)

Ion 77.10 (76.80 to 77.80): VV013543.D (-2432) (-)

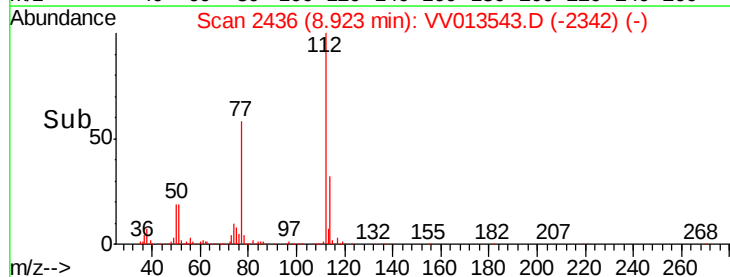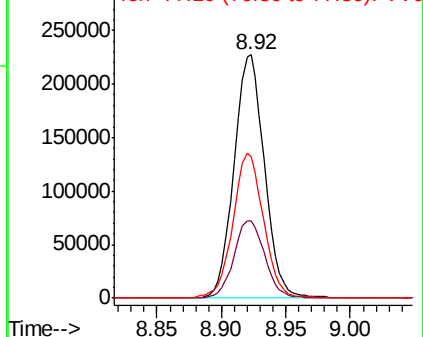

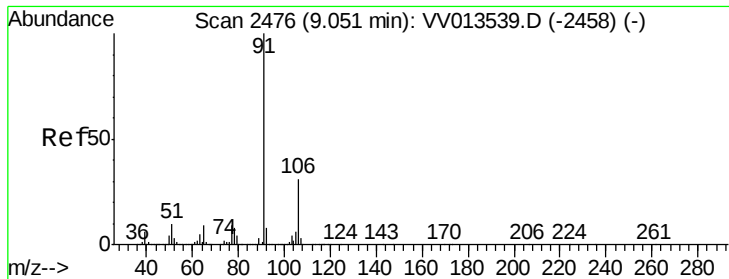

#52

Ethylbenzene

Concen: 0.061 ug/L

RT: 9.05 min Scan# 2477

Delta R.T. 0.00 min

Lab File: VV013543.D

Acq: 08 Nov 2019 16:56

Instrument :

MSVOA_V

ClientSampleId :


F2J00MSD

Tgt Ion: 91 Resp: 8299




Ion Ratio Lower Upper

91 100

106 29.5 21.6 40.0

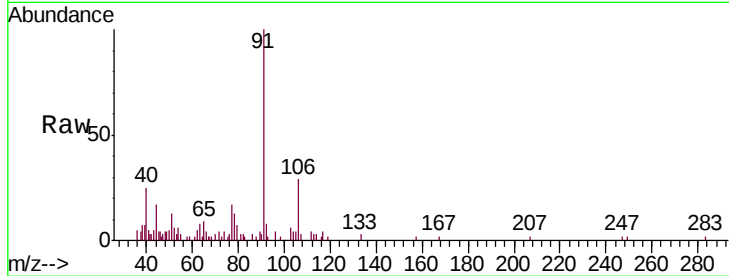

Abundance Ion 91.15 (90.85 to 91.85): VV013539.D (-2458) (-)

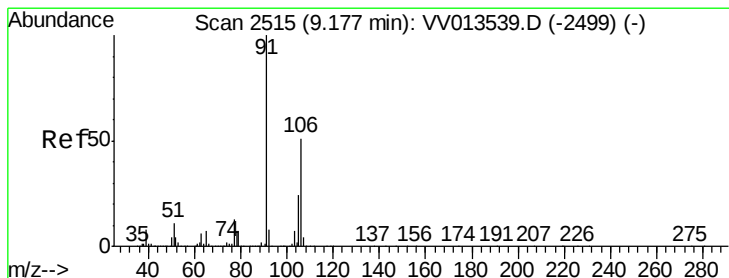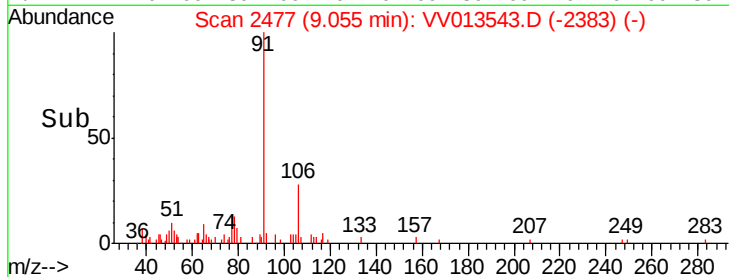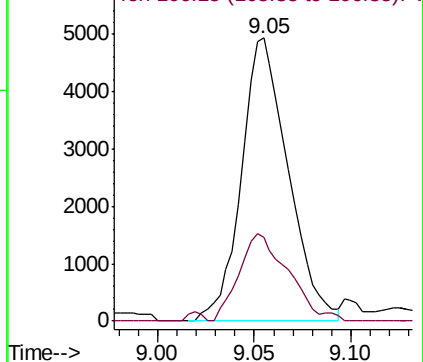

#53

m,p-xylene

Concen: 0.160 ug/L

RT: 9.18 min Scan# 2516

Delta R.T. 0.00 min

Lab File: VV013543.D


Acq: 08 Nov 2019 16:56

Tgt Ion: 106 Resp: 8074



Ion Ratio Lower Upper


106 100

91 218.8 142.0 263.6

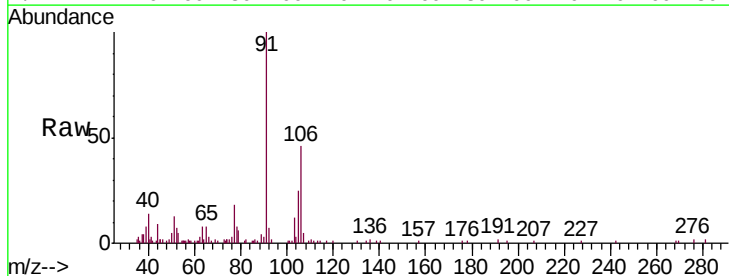

Abundance Ion 106.15 (105.85 to 106.85): VV013539.D (-2499) (-)



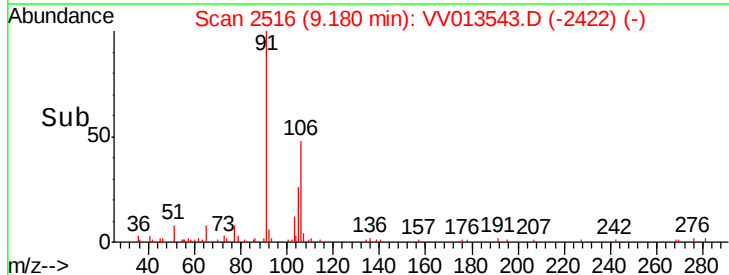
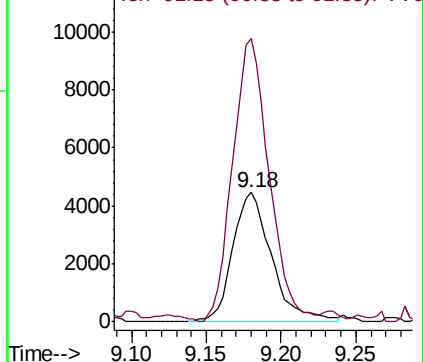


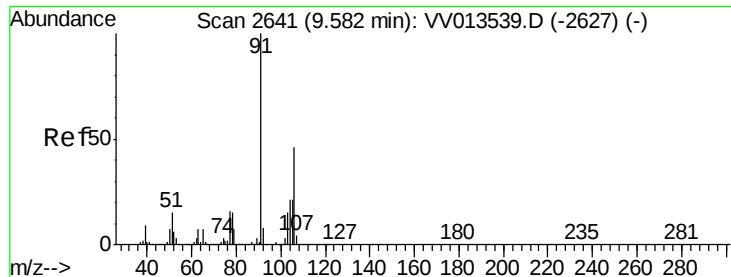

#54
o-xylene
Concen: 0.099 ug/L
RT: 9.59 min Scan# 2642
Delta R.T. 0.00 min
Lab File: VV013543.D
Acq: 08 Nov 2019 16:56




Instrument :
MSVOA_V
ClientSampleId :
F2J00MSD


Tgt Ion:106 Resp: 4821
Ion Ratio Lower Upper
106 100
91 189.5 150.8 280.0

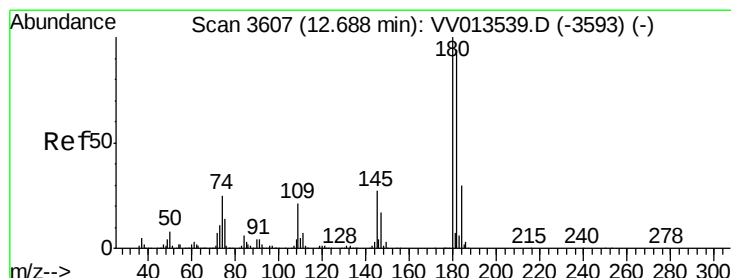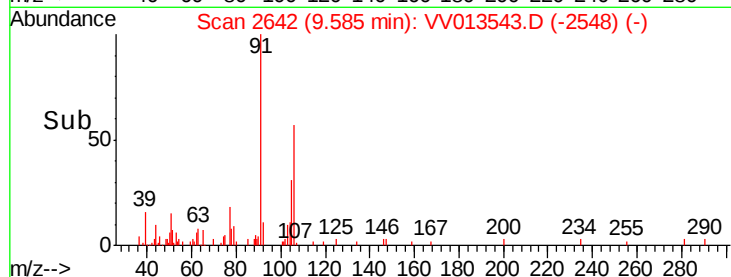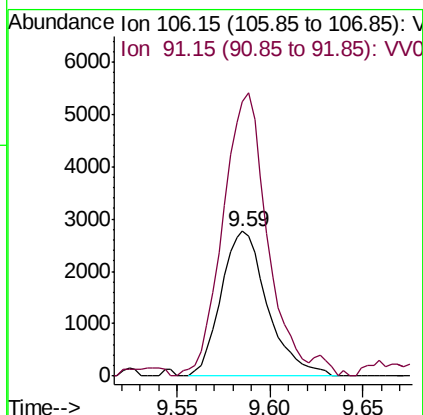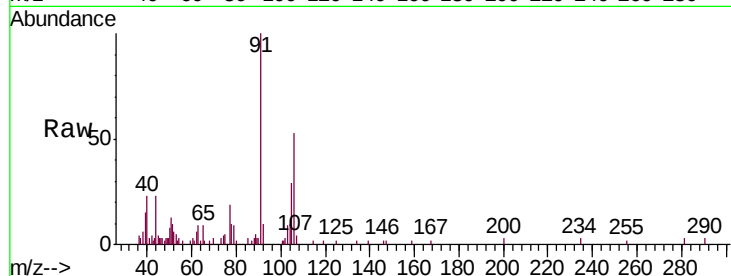

#67
1,3,5-Trichlorobenzene
Concen: 0.059 ug/L
RT: 12.69 min Scan# 3607
Delta R.T. 0.00 min
Lab File: VV013543.D
Acq: 08 Nov 2019 16:56

Tgt Ion:180 Resp: 2892
Ion Ratio Lower Upper
180 100
182 0.0 76.8 115.2#
184 25.9 25.0 37.6
145 0.0 22.1 33.1#

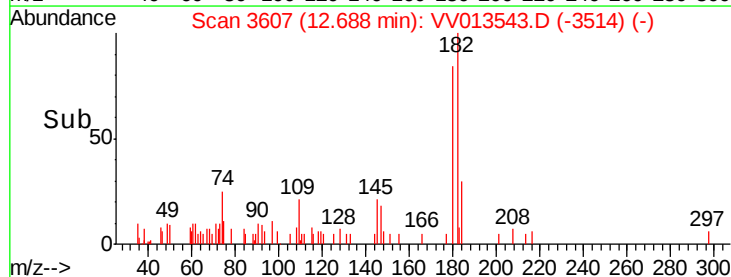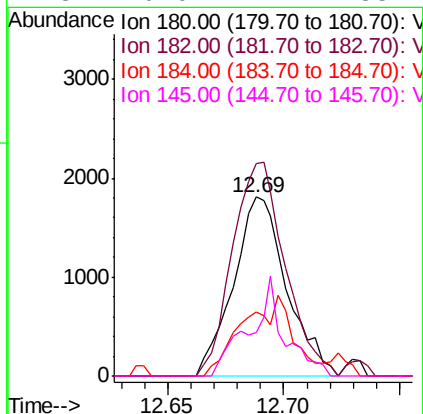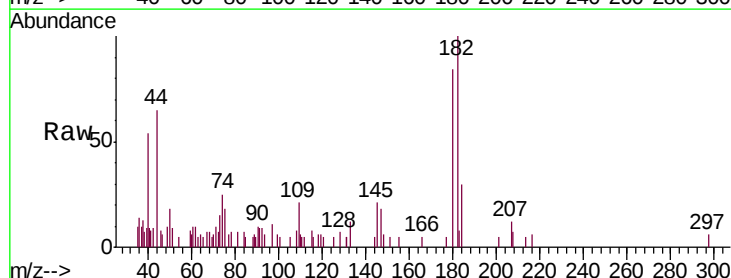


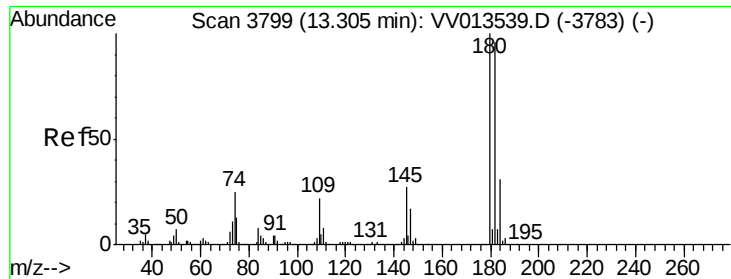




#68
 1,2,4-trichlorobenzene
 Concen: 0.104 ug/L
 RT: 13.31 min Scan# 3799
 Delta R.T. 0.00 min
 Lab File: VV013543.D
 Acq: 08 Nov 2019 16:56

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J00MSD

Tgt Ion:180 Resp: 4070
 Ion Ratio Lower Upper
 180 100
 182 101.9 76.6 115.0
 145 31.4 22.2 33.4

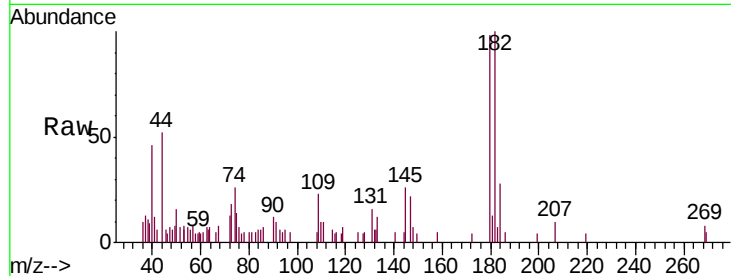


Abundance Ion 179.90 (179.60 to 180.60): V
 Ion 182.00 (181.70 to 182.70): V
 Ion 144.95 (144.65 to 145.65): V

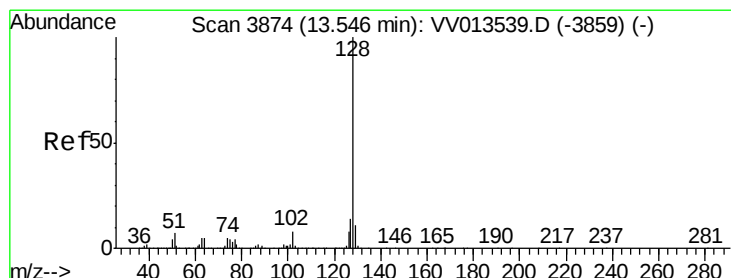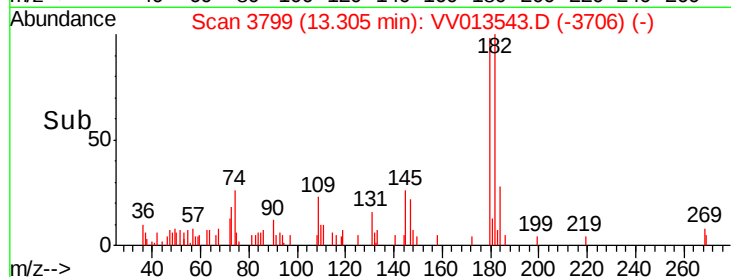
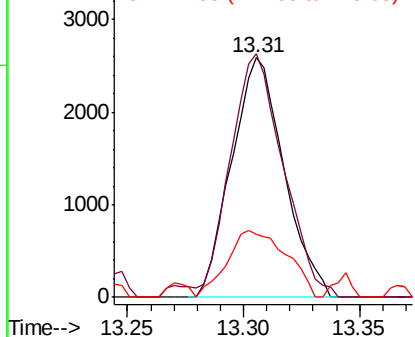



#69
 Naphthalene
 Concen: 18.589 ug/L
 RT: 13.55 min Scan# 3874
 Delta R.T. 0.00 min
 Lab File: VV013543.D
 Acq: 08 Nov 2019 16:56

Tgt Ion:128 Resp: 980744
 Ion Ratio Lower Upper
 128 100
 129 10.7 8.5 12.7
 127 13.3 10.7 16.1

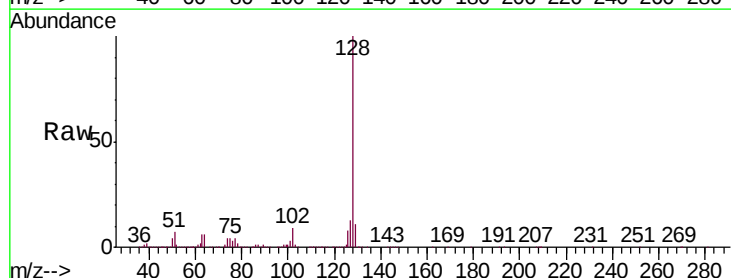

Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 129.00 (128.70 to 129.70): V
 Ion 127.00 (126.70 to 127.70): V

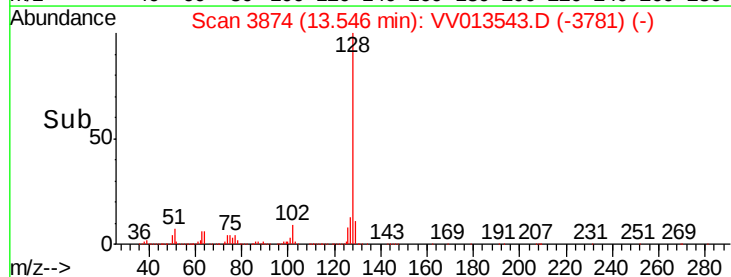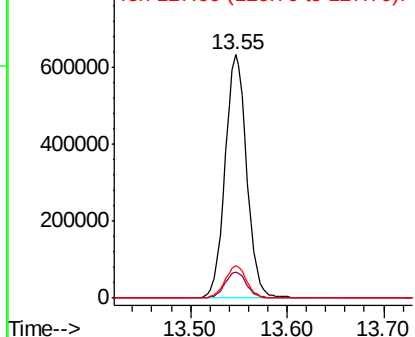

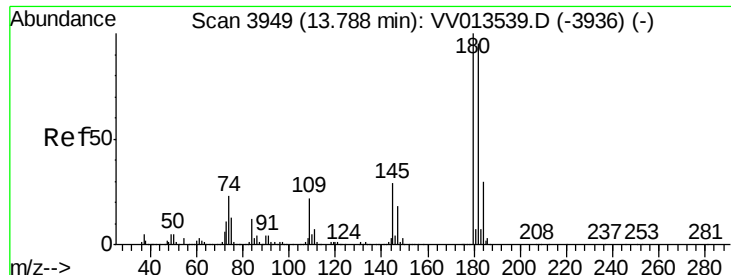

#70
 1,2,3-Trichlorobenzene
 Concen: 0.085 ug/L
 RT: 13.79 min Scan# 3949
 Delta R.T. 0.00 min
 Lab File: VV013543.D
 Acq: 08 Nov 2019 16:56

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J00MSD

Tgt Ion	Ratio	Lower	Upper
180	100		
182	113.8	76.2	114.4
145	27.6	23.2	34.8

