

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013546.D
 Acq On : 08 Nov 2019 18:08
 Operator : SY/MD
 Sample : K5747-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J04

Quant Time: Nov 08 23:57:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 08 22:42:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	415692	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	411365	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	184562	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	85042	4.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.00%
7) Chloroethane-d5	1.58	69	82817	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.40%
11) 1,1-Dichloroethene-d2	2.13	63	107849	3.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.20%
20) 2-Butanone-d5	3.92	46	280014	44.58	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.16%
24) Chloroform-d	4.40	84	210470	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.08	65	118405	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.10	84	394603	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.11	67	136037	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	307264	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
43) trans-1,3-Dichloropropene-	7.66	79	47030	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.13	63	183121	42.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.60%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	96271	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	162196	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.18	43	35410	9.293 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013546.D
Acq On : 08 Nov 2019 18:08
Operator : SY/MD
Sample : K5747-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J04

Quant Time: Nov 08 23:57:36 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

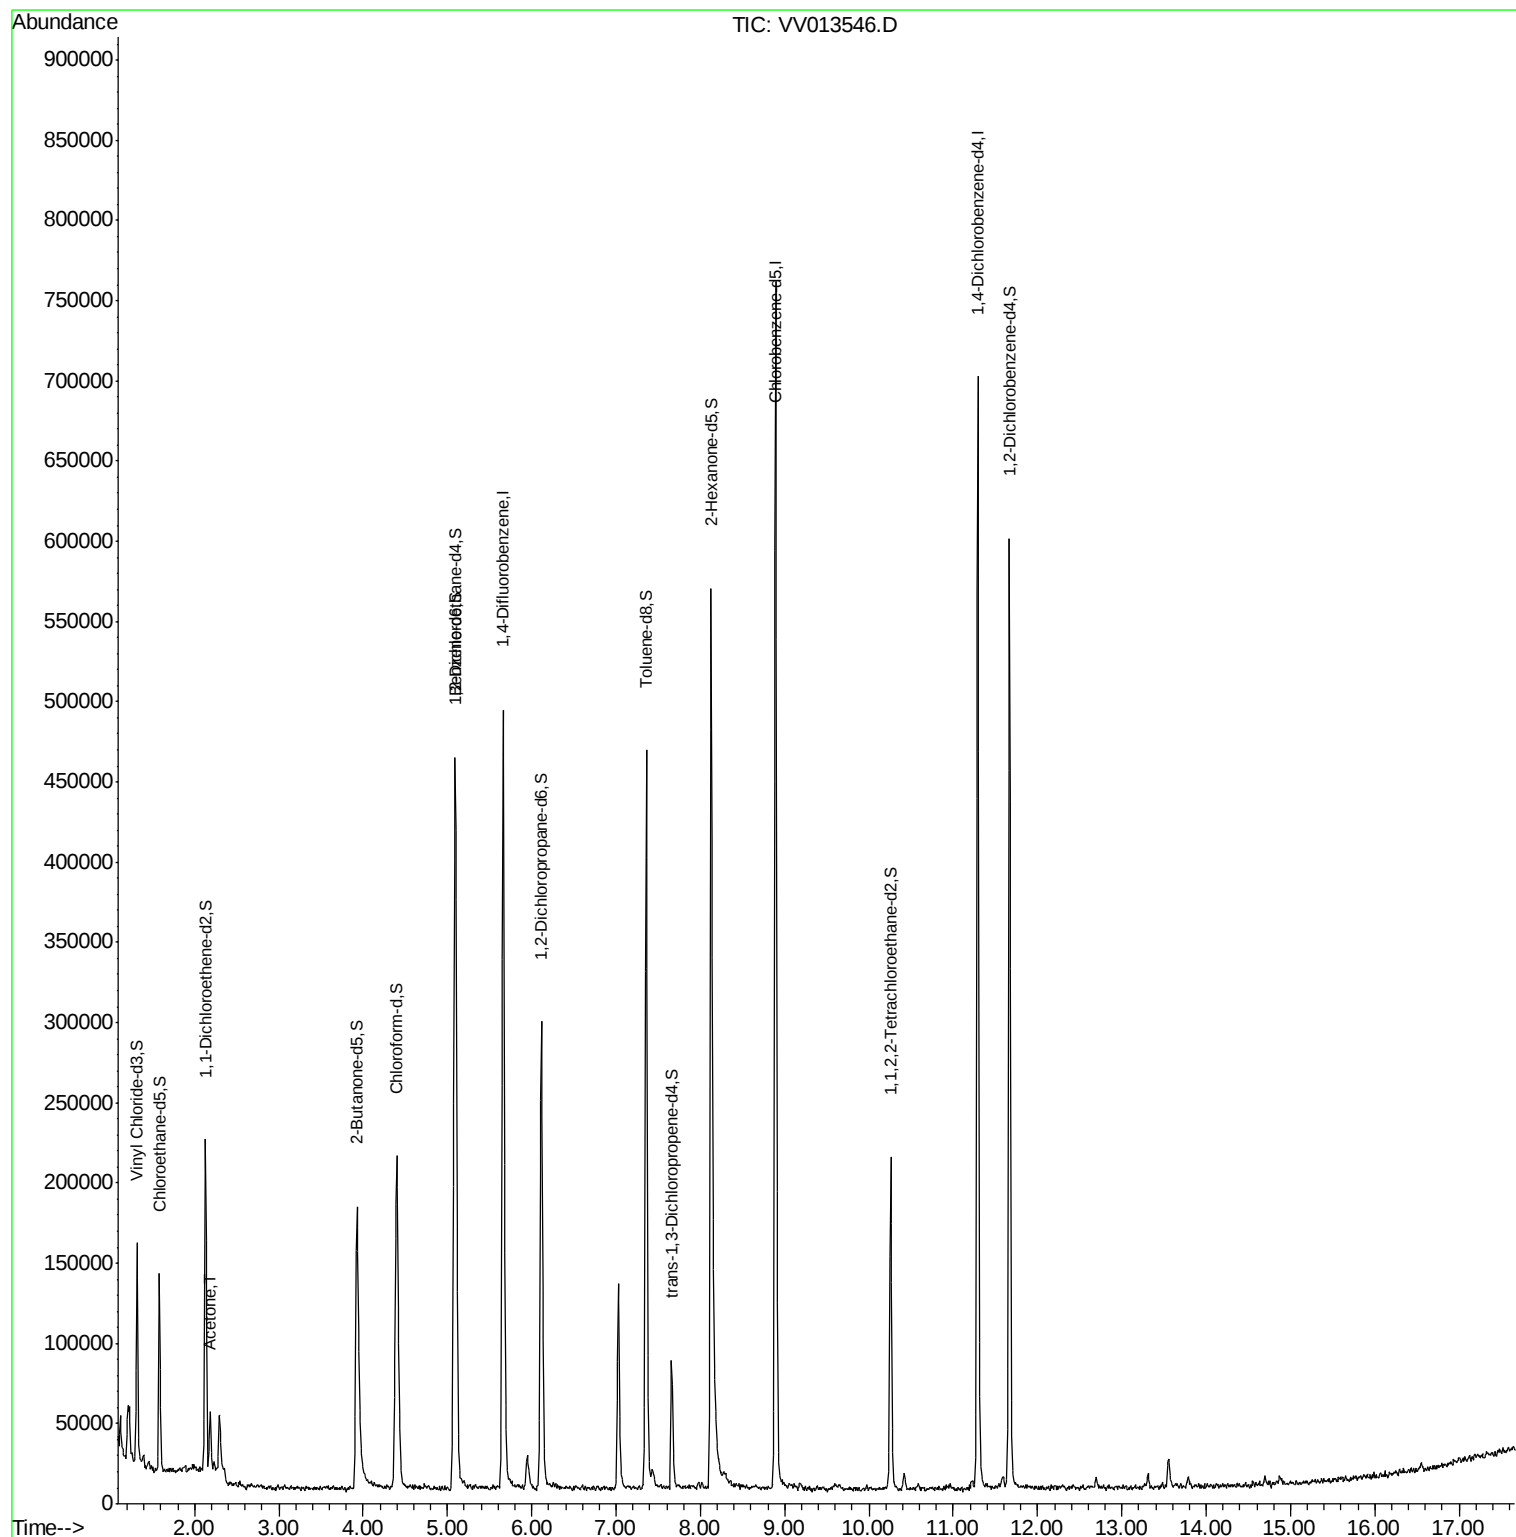

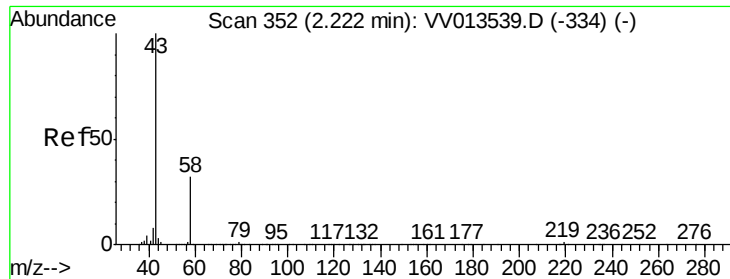

#13

Acetone

Concen: 9.293 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV013546.D

Acq: 08 Nov 2019 18:08


Instrument :
MSVOA_V
ClientSampleId :
F2J04

Tot Ion: 43 Resp: 35410

Ion Ratio Lower Upper

43 100

58 34.2 0.0 60.8

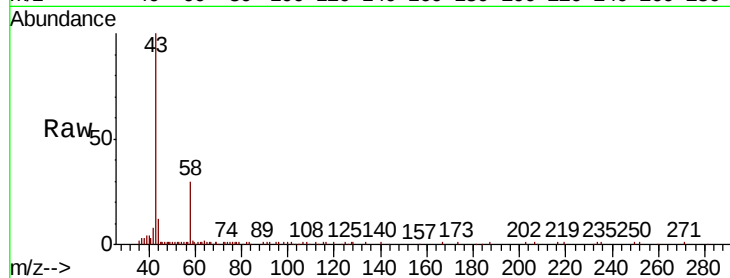

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

