

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013547.D
 Acq On : 08 Nov 2019 18:32
 Operator : SY/MD
 Sample : K5747-08
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J06

Quant Time: Nov 09 00:00:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 08 22:42:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	386513	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	384914	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	176262	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	83058	5.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.00%
7) Chloroethane-d5	1.58	69	77228	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.80%
11) 1,1-Dichloroethene-d2	2.13	63	104847	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	3.93	46	280896	48.10	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.20%
24) Chloroform-d	4.40	84	208014	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.08	65	118903	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.60%
32) Benzene-d6	5.10	84	384442	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.11	67	135250	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.36	98	299715	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	7.66	79	45140	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.13	63	171554	42.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.70%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	91279	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	159171	5.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.20%


Target Compounds					Ovalue
13) Acetone	2.18	43	25485	7.193 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013547.D
Acq On : 08 Nov 2019 18:32
Operator : SY/MD
Sample : K5747-08
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J06

Quant Time: Nov 09 00:00:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

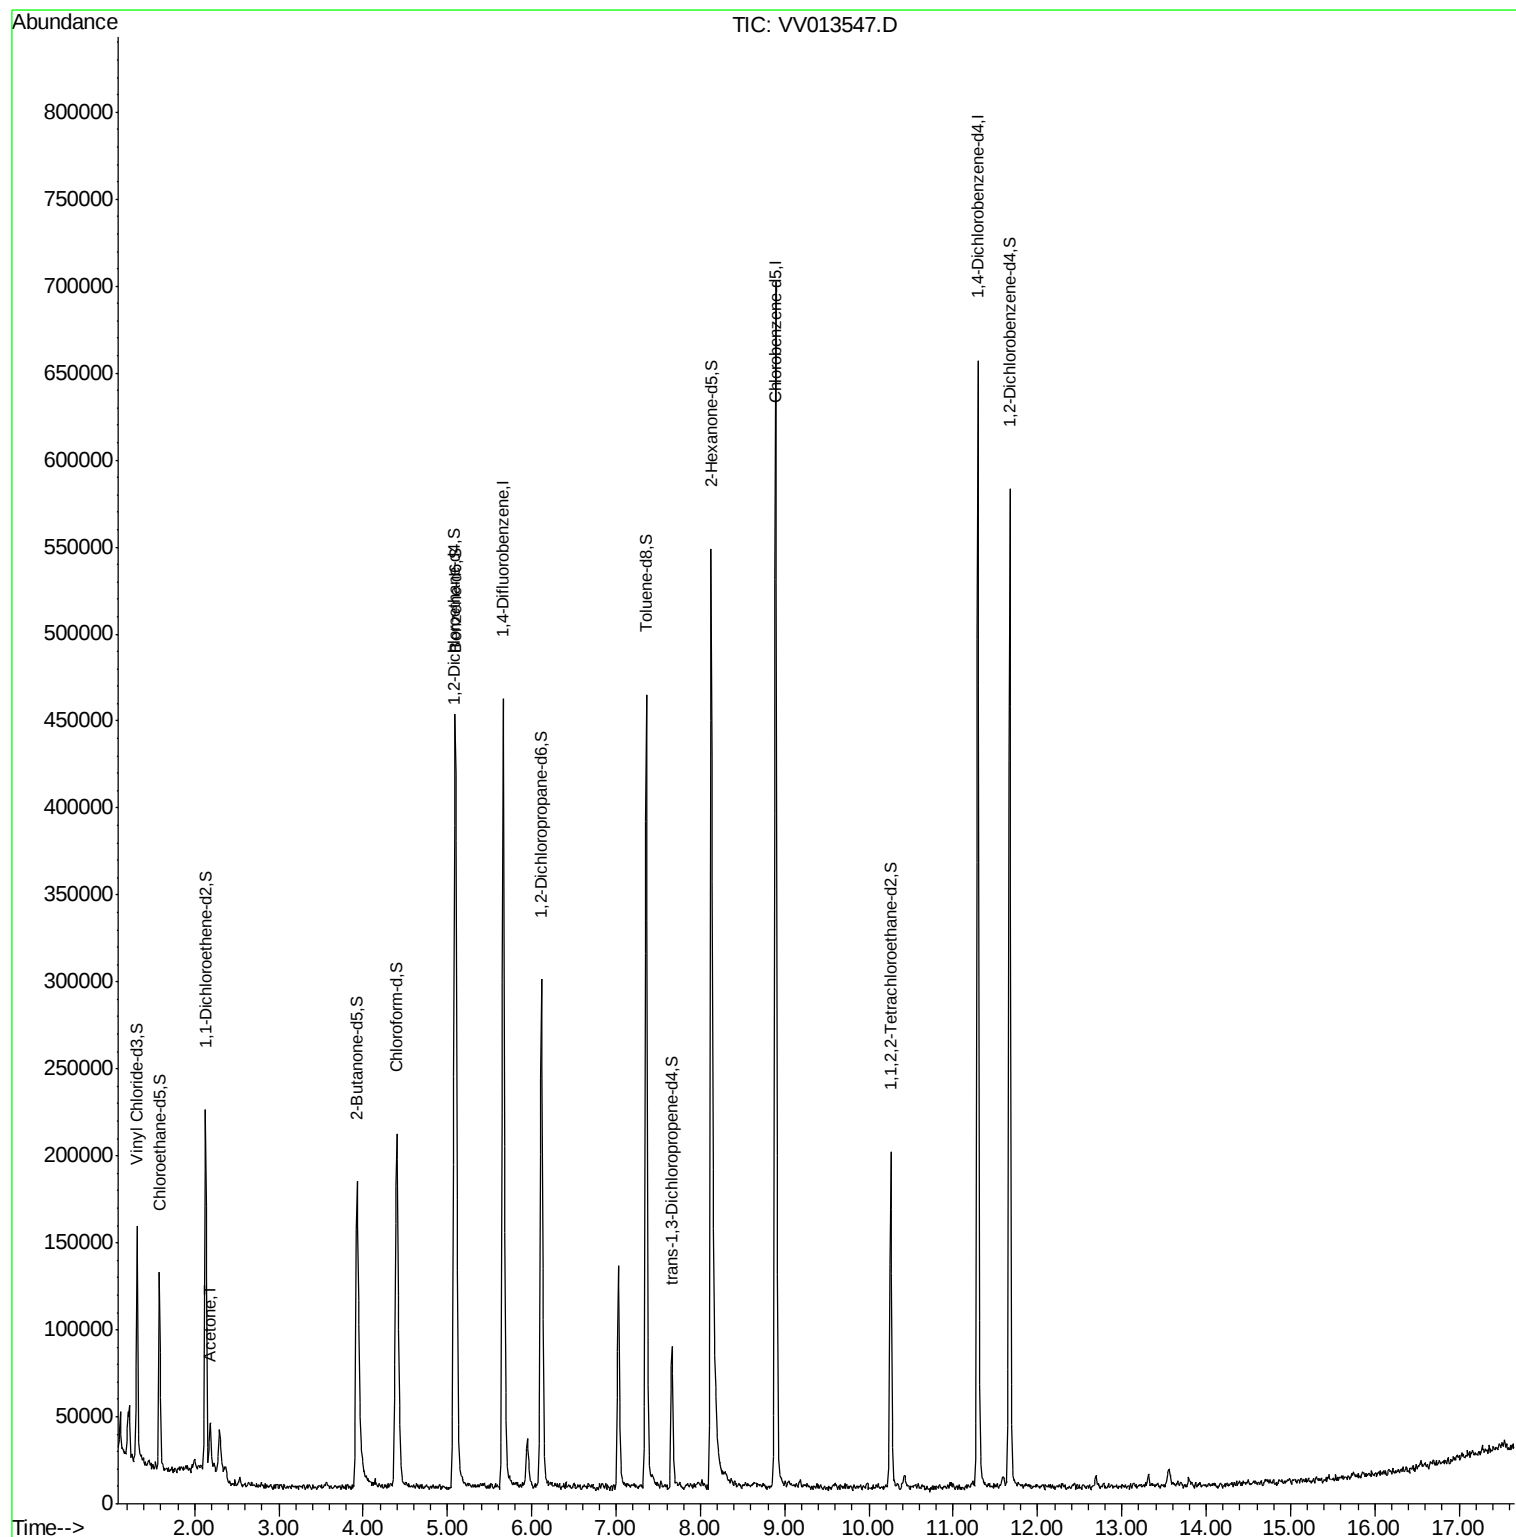

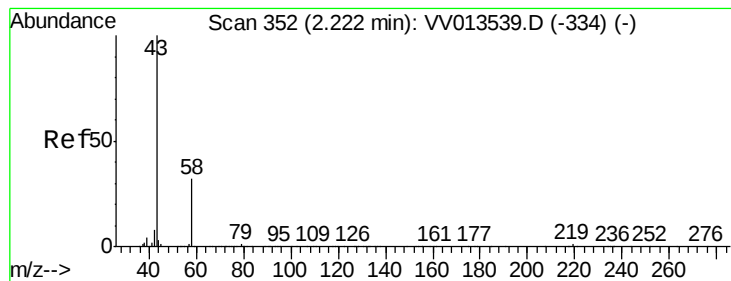

#13
 Acetone
 Concen: 7.193 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. -0.04 min
 Lab File: VV013547.D
 Acq: 08 Nov 2019 18:32

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J06

Tot Ion: 43 Resp: 25485
 Ion Ratio Lower Upper
 43 100
 58 32.0 0.0 60.8

