

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013552.D
 Acq On : 08 Nov 2019 20:32
 Operator : SY/MD
 Sample : K5718-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE9S5

Quant Time: Nov 09 00:53:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 08 22:42:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	379787	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	385457	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	165913	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	79834	4.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.80%
7) Chloroethane-d5	1.58	69	78808	5.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.80%
11) 1,1-Dichloroethene-d2	2.13	63	105941	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	3.93	46	313446	54.62	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.24%
24) Chloroform-d	4.40	84	212561	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.08	65	116478	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.20%
32) Benzene-d6	5.10	84	383754	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.11	67	137316	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.36	98	296603	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.66	79	45554	4.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.00%
46) 2-Hexanone-d5	8.13	63	184709	45.54	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.08%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	102741	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	152135	5.55	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.00%


Target Compounds					Ovalue
13) Acetone	2.18	43	7684	2.207 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013552.D
Acq On : 08 Nov 2019 20:32
Operator : SY/MD
Sample : K5718-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE9S5

Quant Time: Nov 09 00:53:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

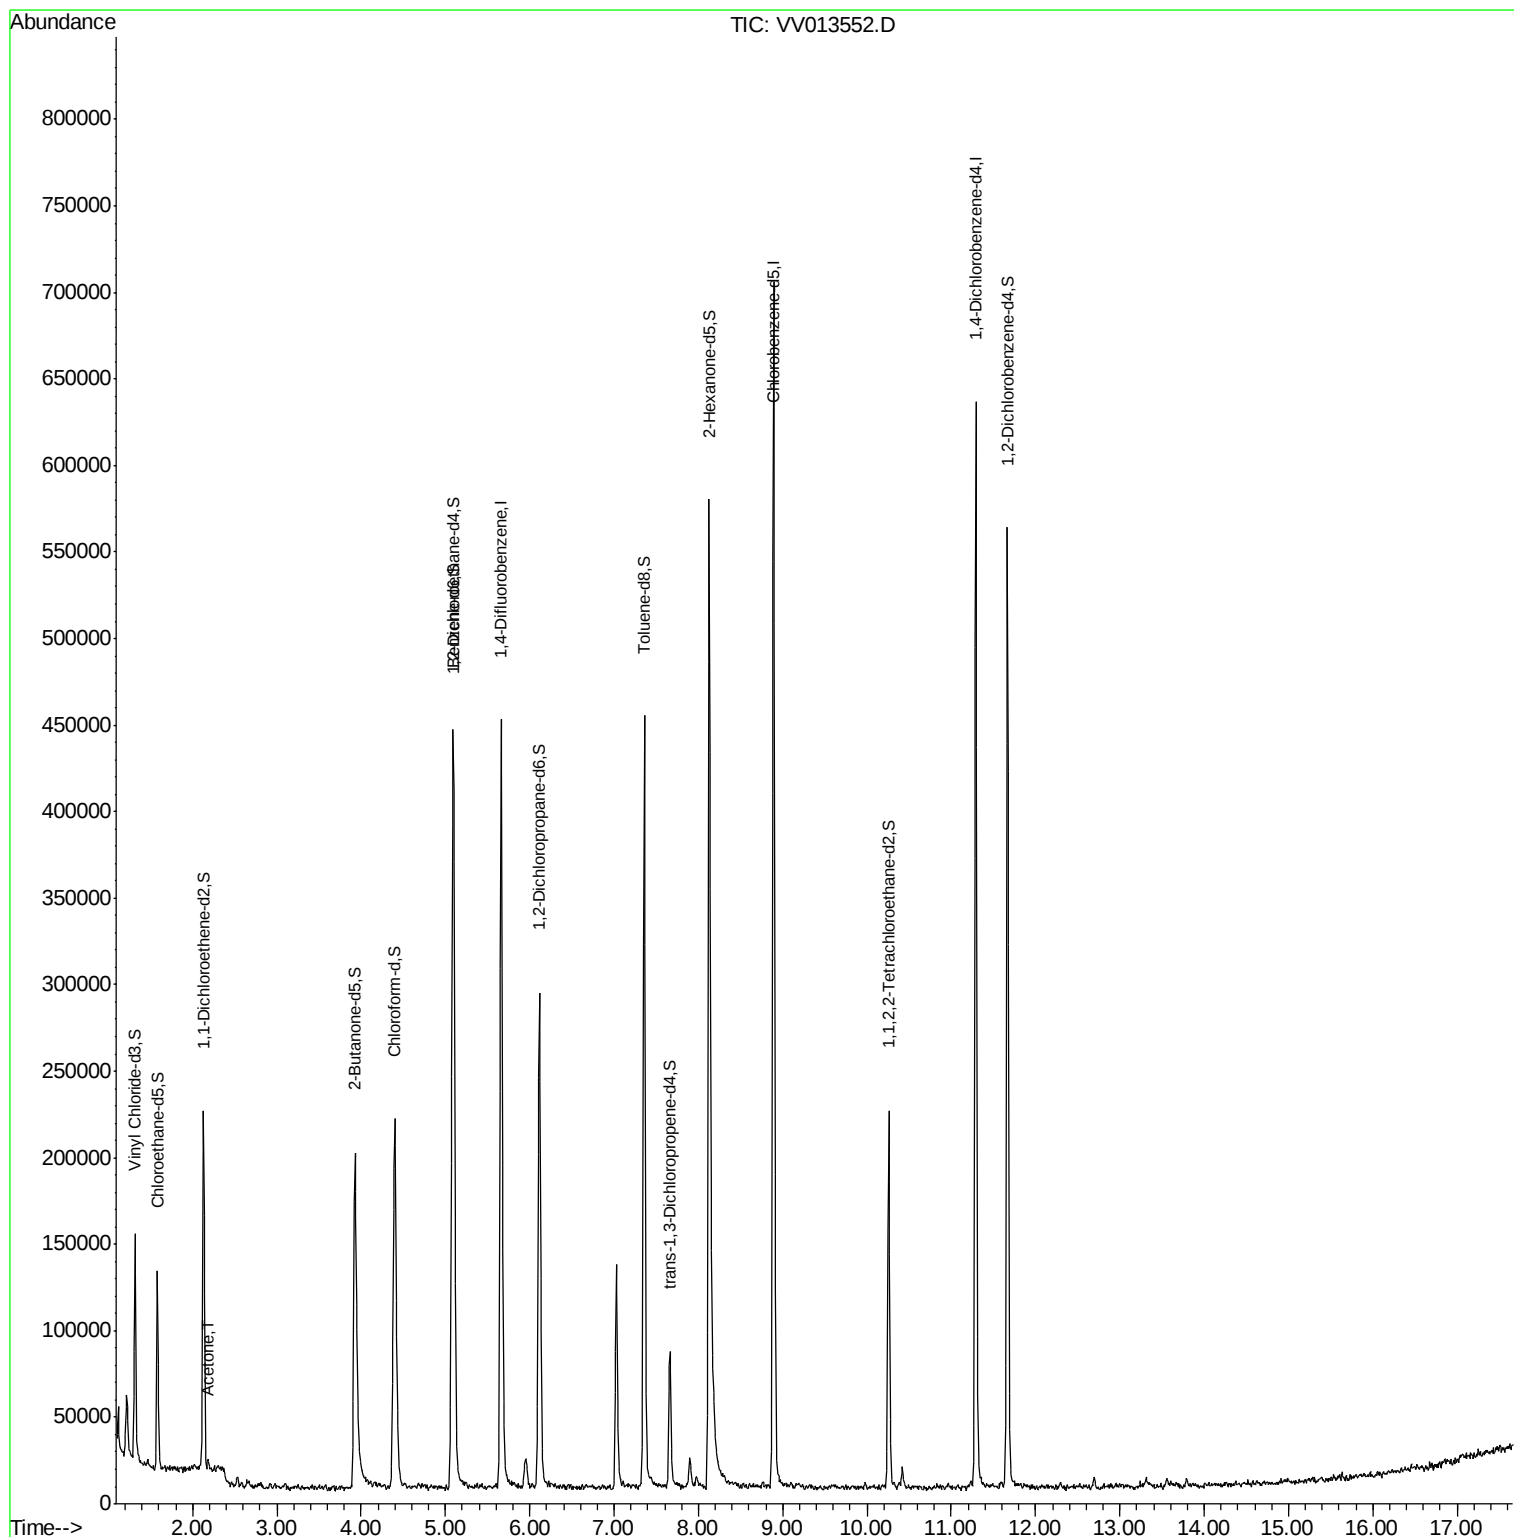

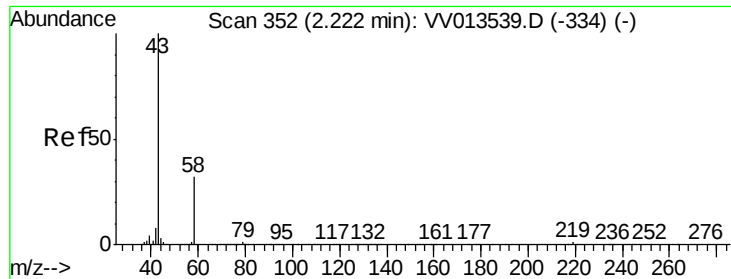

#13

Acetone

Concen: 2.207 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV013552.D

Acq: 08 Nov 2019 20:32

Instrument :
MSVOA_V
ClientSampleId :
BE9S5

Tot Ion: 43 Resp: 7684

Ion Ratio Lower Upper

43 100

58 37.7 0.0 60.8

