

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013553.D
 Acq On : 08 Nov 2019 20:57
 Operator : SY/MD
 Sample : K5718-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE9S6

Quant Time: Nov 09 00:56:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 08 22:42:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	365839	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	372823	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	163625	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80725	5.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.60%
7) Chloroethane-d5	1.58	69	77222	5.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.80%
11) 1,1-Dichloroethene-d2	2.13	63	102011	3.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.80%
20) 2-Butanone-d5	3.93	46	296260	53.60	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.20%
24) Chloroform-d	4.40	84	197508	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.08	65	113832	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.80%
32) Benzene-d6	5.10	84	370003	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.12	67	128330	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.36	98	281606	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	7.66	79	45053	4.60	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.00%
46) 2-Hexanone-d5	8.13	63	171783	43.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.58%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	94186	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	148436	5.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.80%


Target Compounds				Ovalue
13) Acetone	2.19	43	8188	2.442 ug/L 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013553.D
Acq On : 08 Nov 2019 20:57
Operator : SY/MD
Sample : K5718-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE9S6

Quant Time: Nov 09 00:56:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

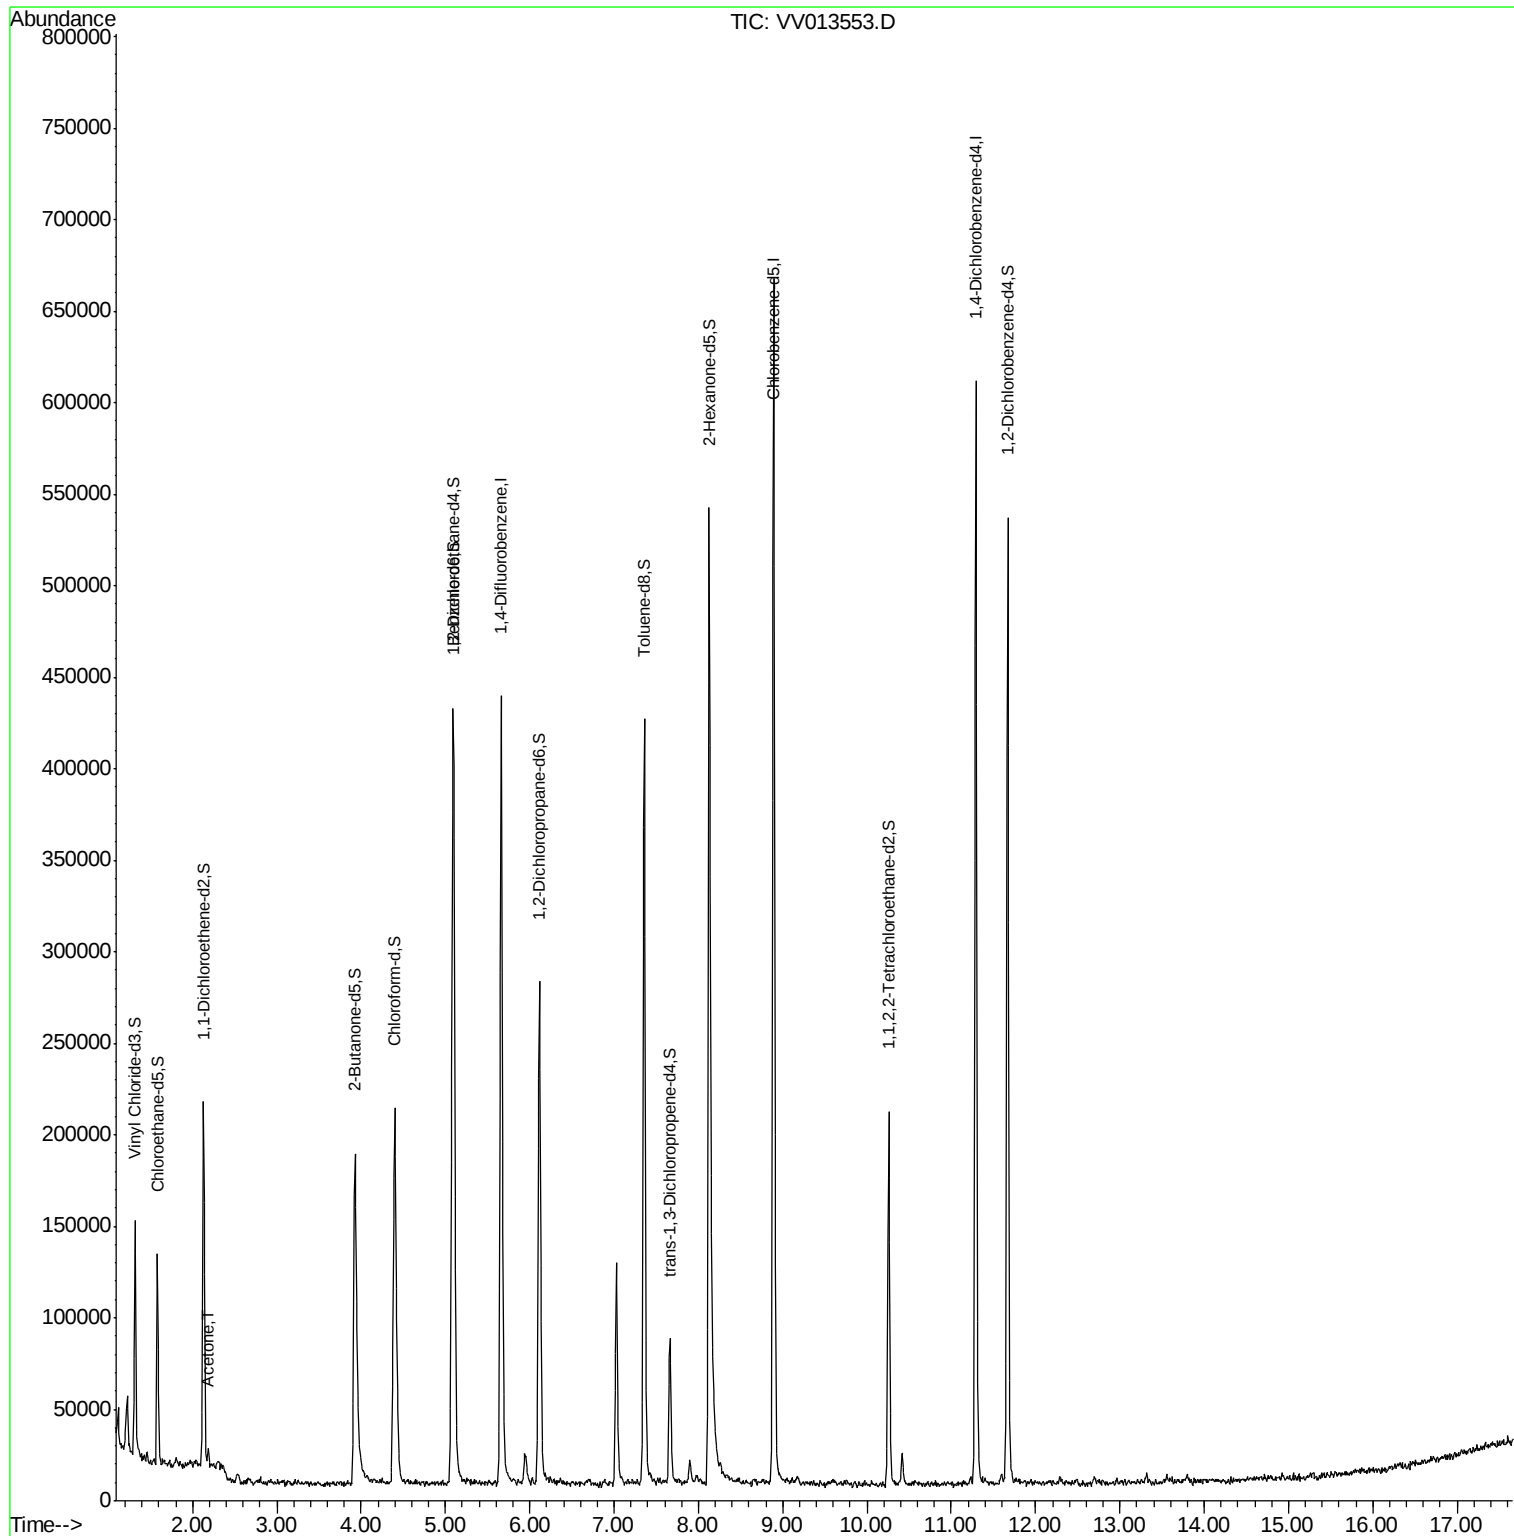

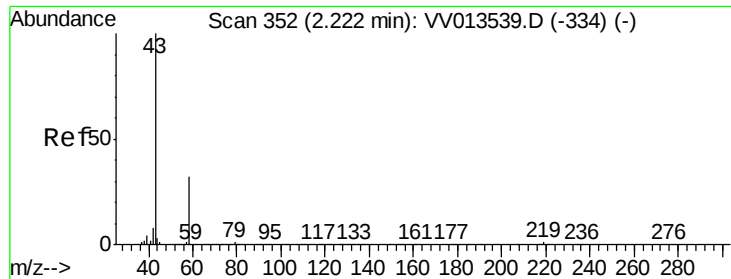

#13

Acetone

Concen: 2.442 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.04 min

Lab File: VV013553.D

Acq: 08 Nov 2019 20:57

Instrument :
MSVOA_V
ClientSampleId :
BE9S6

Tot Ion: 43 Resp: 8188

Ion Ratio Lower Upper

43 100

58 35.6 0.0 60.8

