

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013554.D
 Acq On : 08 Nov 2019 21:21
 Operator : SY/MD
 Sample : K5718-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE9S7

Quant Time: Nov 09 00:58:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 08 22:42:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	373683	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	382673	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	169090	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	79922	5.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.40%
7) Chloroethane-d5	1.58	69	74882	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.00%
11) 1,1-Dichloroethene-d2	2.13	63	101884	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	3.94	46	312859	55.41	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.82%
24) Chloroform-d	4.40	84	204866	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
26) 1,2-Dichloroethane-d4	5.08	65	115485	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.00%
32) Benzene-d6	5.10	84	372619	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.12	67	131847	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.36	98	283785	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.66	79	44886	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.13	63	174677	43.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.76%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	101335	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	148145	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	8418	2.458 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013554.D
Acq On : 08 Nov 2019 21:21
Operator : SY/MD
Sample : K5718-05
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE9S7

Quant Time: Nov 09 00:58:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 08 22:42:17 2019
Response via : Initial Calibration

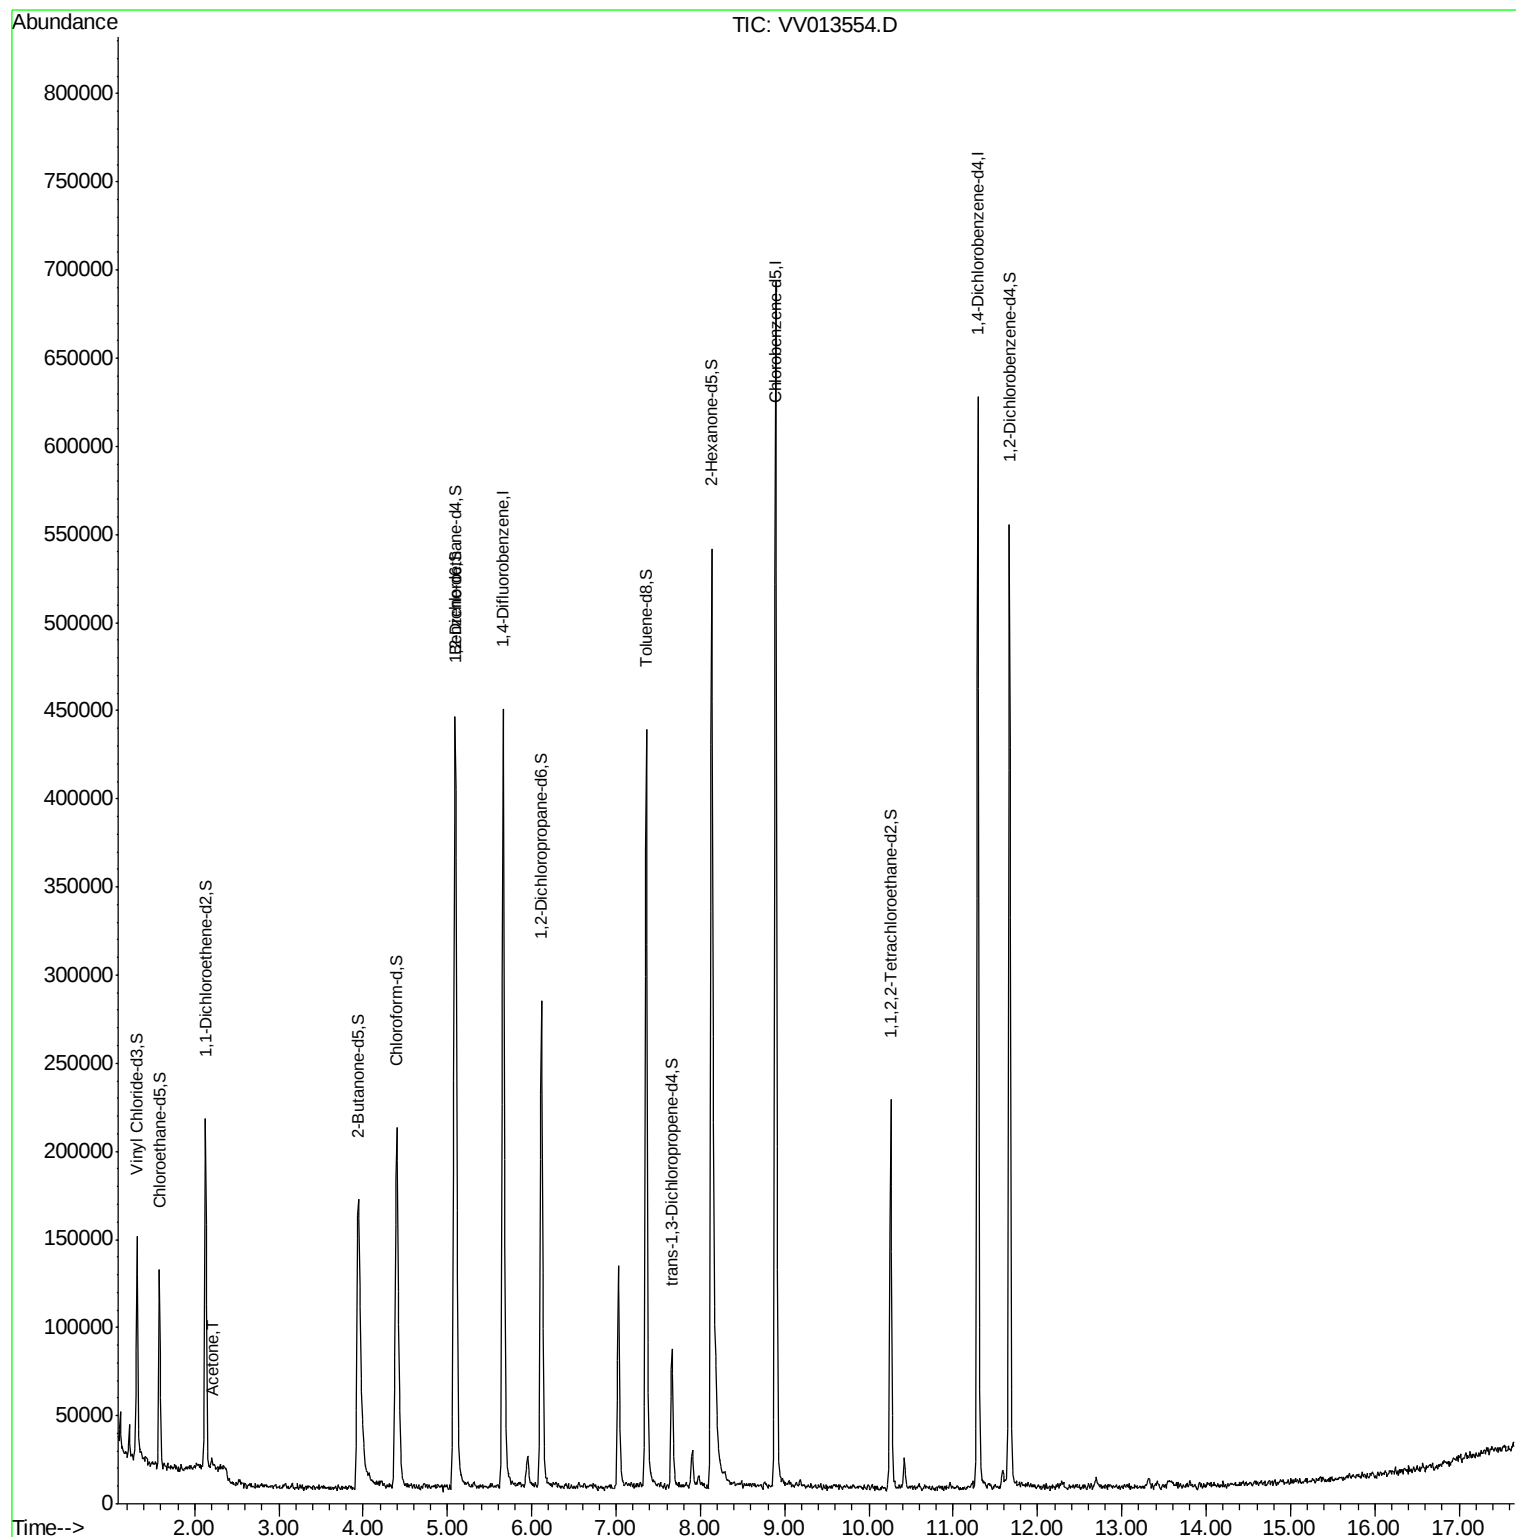

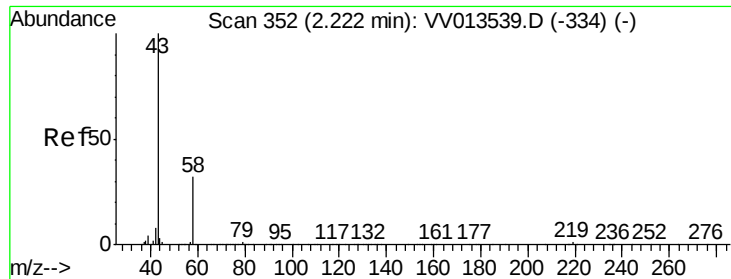

#13

Acetone

Concen: 2.458 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.02 min

Lab File: VV013554.D

Acq: 08 Nov 2019 21:21


Instrument :
MSVOA_V
ClientSampleId :
BE9S7

Tot Ion: 43 Resp: 8418

Ion Ratio Lower Upper

43 100

58 42.3 0.0 60.8

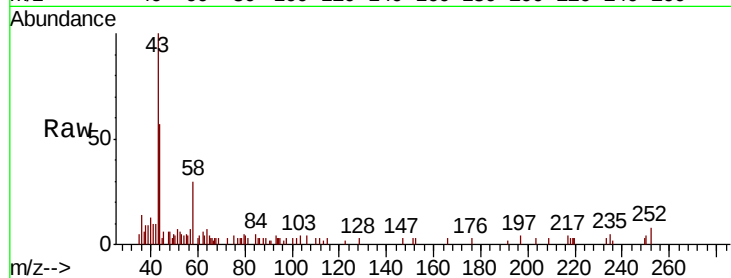

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

2.21

5000

4000

3000

2000

1000

0

Time-->

2.15 2.20 2.25

