

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013564.D
 Acq On : 09 Nov 2019 02:09
 Operator : SY/MD
 Sample : K5747-14
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J08

Quant Time: Nov 09 04:53:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 09 04:21:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	371083	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	379752	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	165953	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77652	4.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.20%
7) Chloroethane-d5	1.58	69	76341	5.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.00%
11) 1,1-Dichloroethene-d2	2.13	63	102983	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	3.95	46	290028	51.73	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.46%
24) Chloroform-d	4.40	84	214538	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
26) 1,2-Dichloroethane-d4	5.08	65	115712	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.00%
32) Benzene-d6	5.10	84	374676	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.11	67	134038	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.36	98	286108	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
43) trans-1,3-Dichloropropene-	7.66	79	42299	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
46) 2-Hexanone-d5	8.13	63	159094	39.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.62%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	94115	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	151151	5.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	33152	9.747 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013564.D
Acq On : 09 Nov 2019 02:09
Operator : SY/MD
Sample : K5747-14
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J08

Quant Time: Nov 09 04:53:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 09 04:21:29 2019
Response via : Initial Calibration

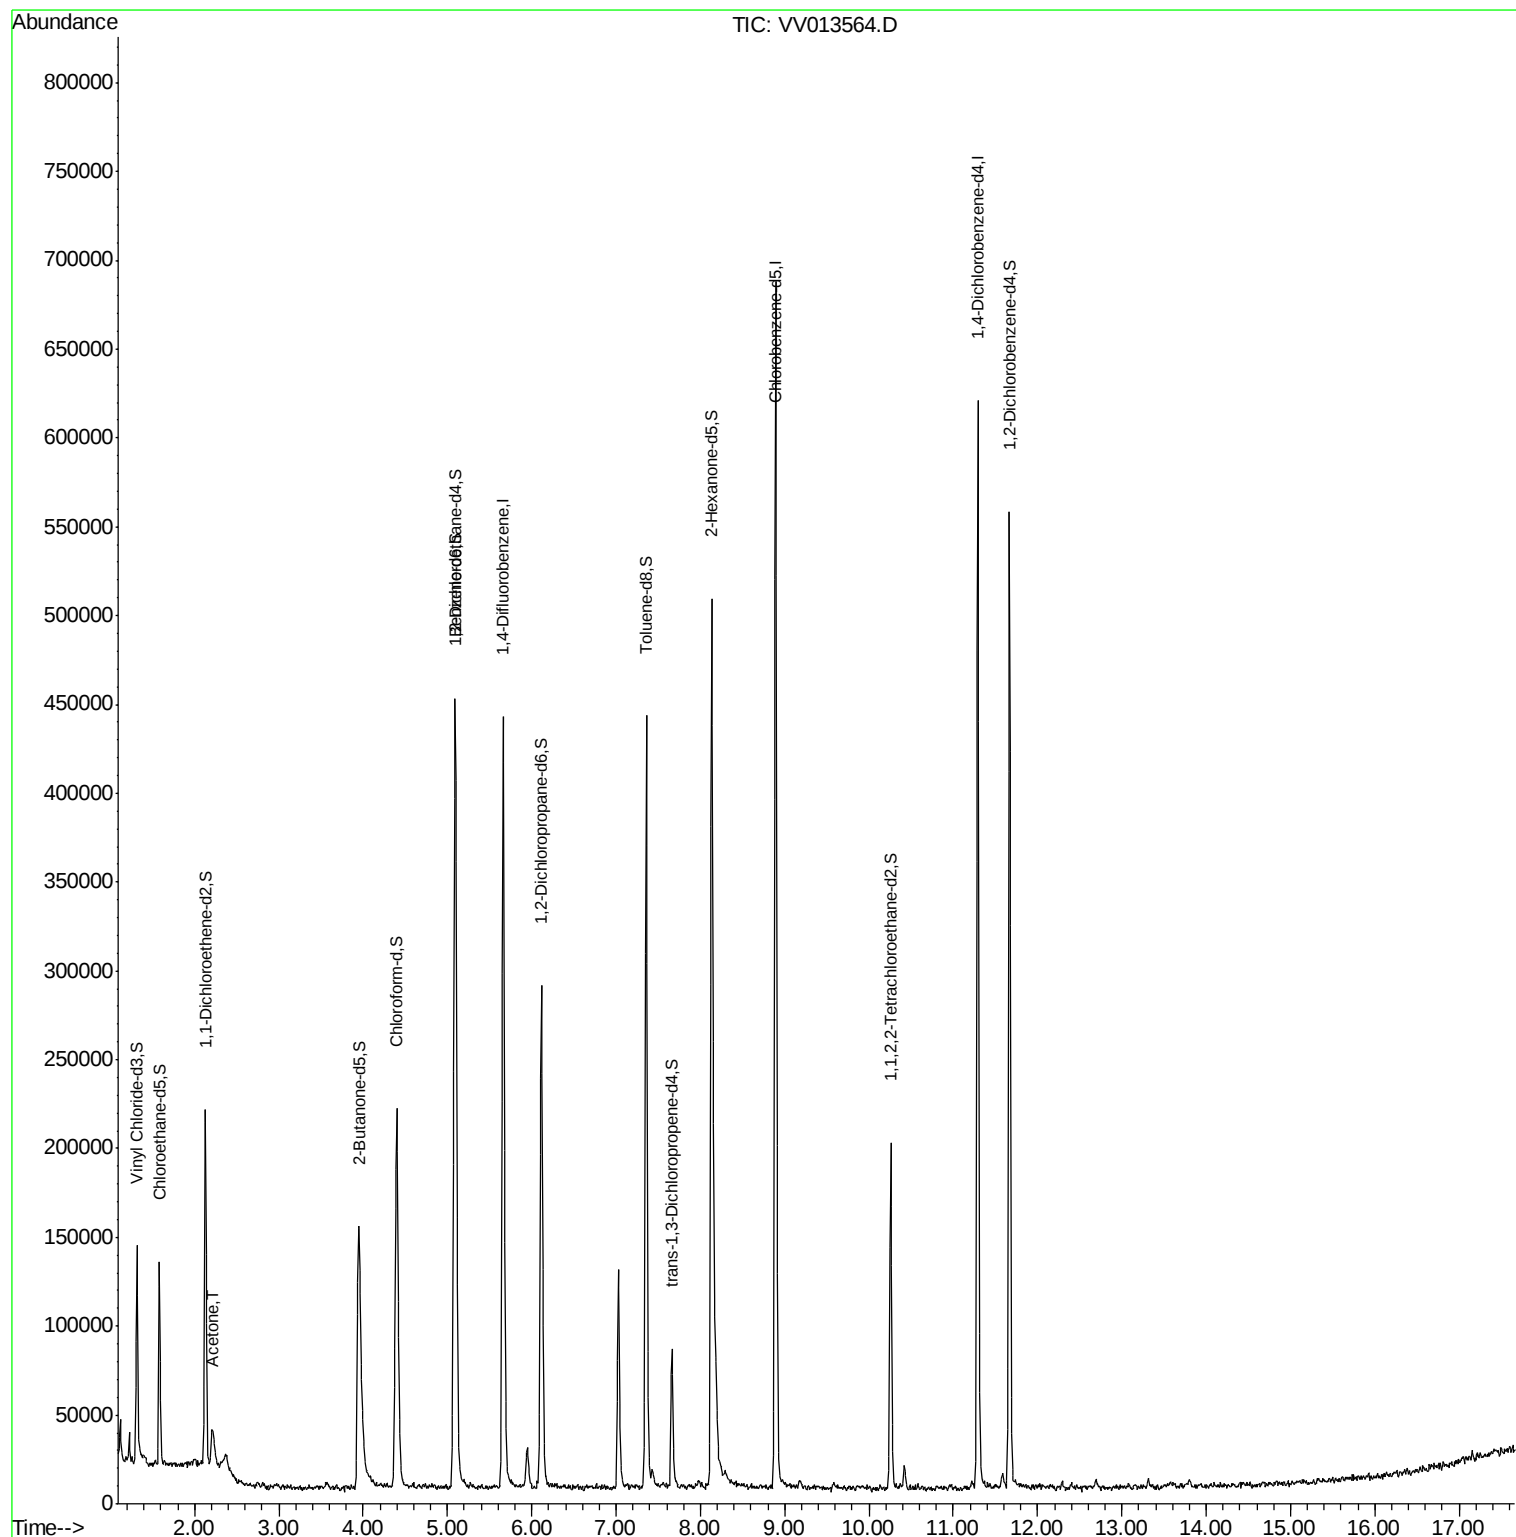

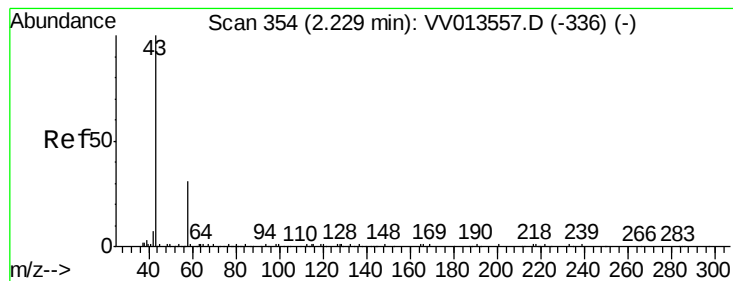

#13

Acetone

Concen: 9.747 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.02 min

Lab File: VV013564.D

Acq: 09 Nov 2019 02:09

Instrument :
MSVOA_V
ClientSampleId :
F2J08

Tot Ion: 43 Resp: 33152

Ion Ratio Lower Upper

43 100

58 31.7 0.0 60.8

