

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013566.D
 Acq On : 09 Nov 2019 02:57
 Operator : SY/MD
 Sample : K5747-16
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J11

Quant Time: Nov 09 04:57:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 09 04:21:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	381706	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	382471	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	171542	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	81464	5.06	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.20%
7) Chloroethane-d5	1.58	69	76774	5.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.40%
11) 1,1-Dichloroethene-d2	2.13	63	104211	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	3.92	46	305983	53.05	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.10%
24) Chloroform-d	4.40	84	200172	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.08	65	114225	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
32) Benzene-d6	5.10	84	370847	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.11	67	130627	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.36	98	276261	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloropropene-	7.66	79	43736	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.13	63	173539	43.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.24%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	94648	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	145172	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%


Target Compounds					Ovalue
13) Acetone	2.18	43	24568	7.022 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013566.D
Acq On : 09 Nov 2019 02:57
Operator : SY/MD
Sample : K5747-16
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J11

Quant Time: Nov 09 04:57:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 09 04:21:29 2019
Response via : Initial Calibration

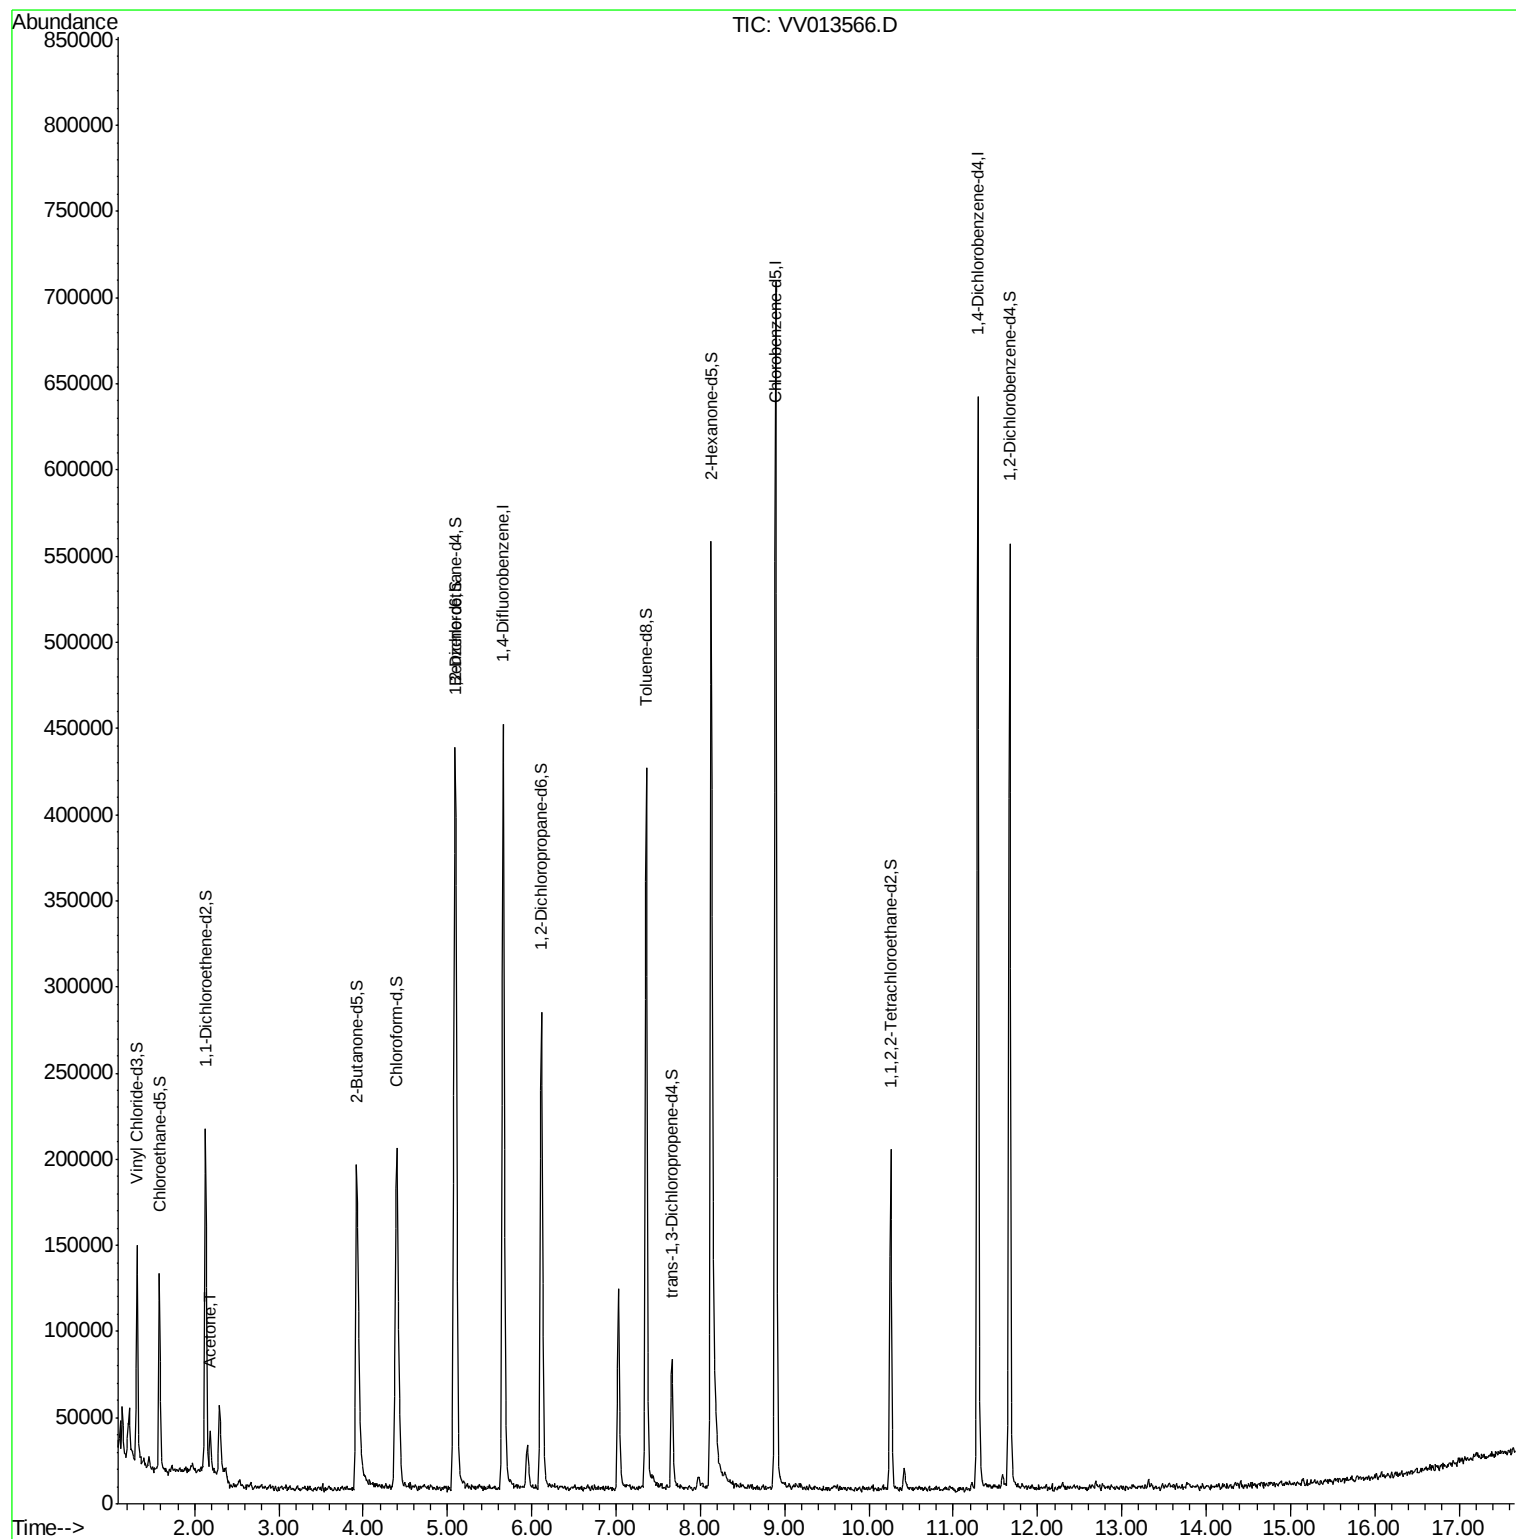

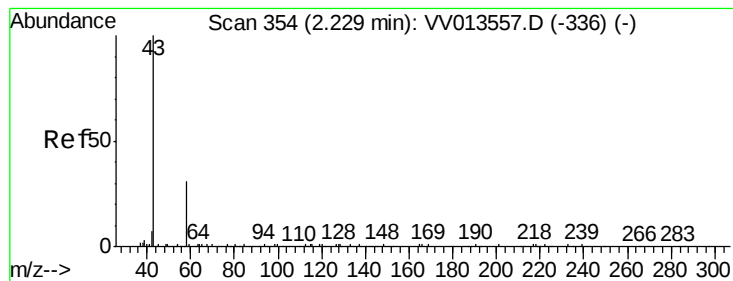

#13

Acetone

Concen: 7.022 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV013566.D

Acq: 09 Nov 2019 02:57

Instrument :
MSVOA_V
ClientSampleId :
F2J11

Tot Ion: 43 Resp: 24568

Ion Ratio Lower Upper

43 100

58 32.0 0.0 60.8

