

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013567.D
 Acq On : 09 Nov 2019 03:21
 Operator : SY/MD
 Sample : K5747-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J12

Quant Time: Nov 09 04:59:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 09 04:21:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	365120	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	372625	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	161959	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	76965	5.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.00%
7) Chloroethane-d5	1.58	69	76213	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.13	63	101100	3.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.40%
20) 2-Butanone-d5	3.92	46	291747	52.88	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.76%
24) Chloroform-d	4.40	84	192281	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	5.08	65	109967	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.10	84	361085	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.11	67	131359	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	7.36	98	276623	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	7.66	79	42205	4.31	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.20%
46) 2-Hexanone-d5	8.13	63	167298	42.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	89882	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	146515	5.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	23377	6.985 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013567.D
Acq On : 09 Nov 2019 03:21
Operator : SY/MD
Sample : K5747-17
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J12

Quant Time: Nov 09 04:59:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 09 04:21:29 2019
Response via : Initial Calibration

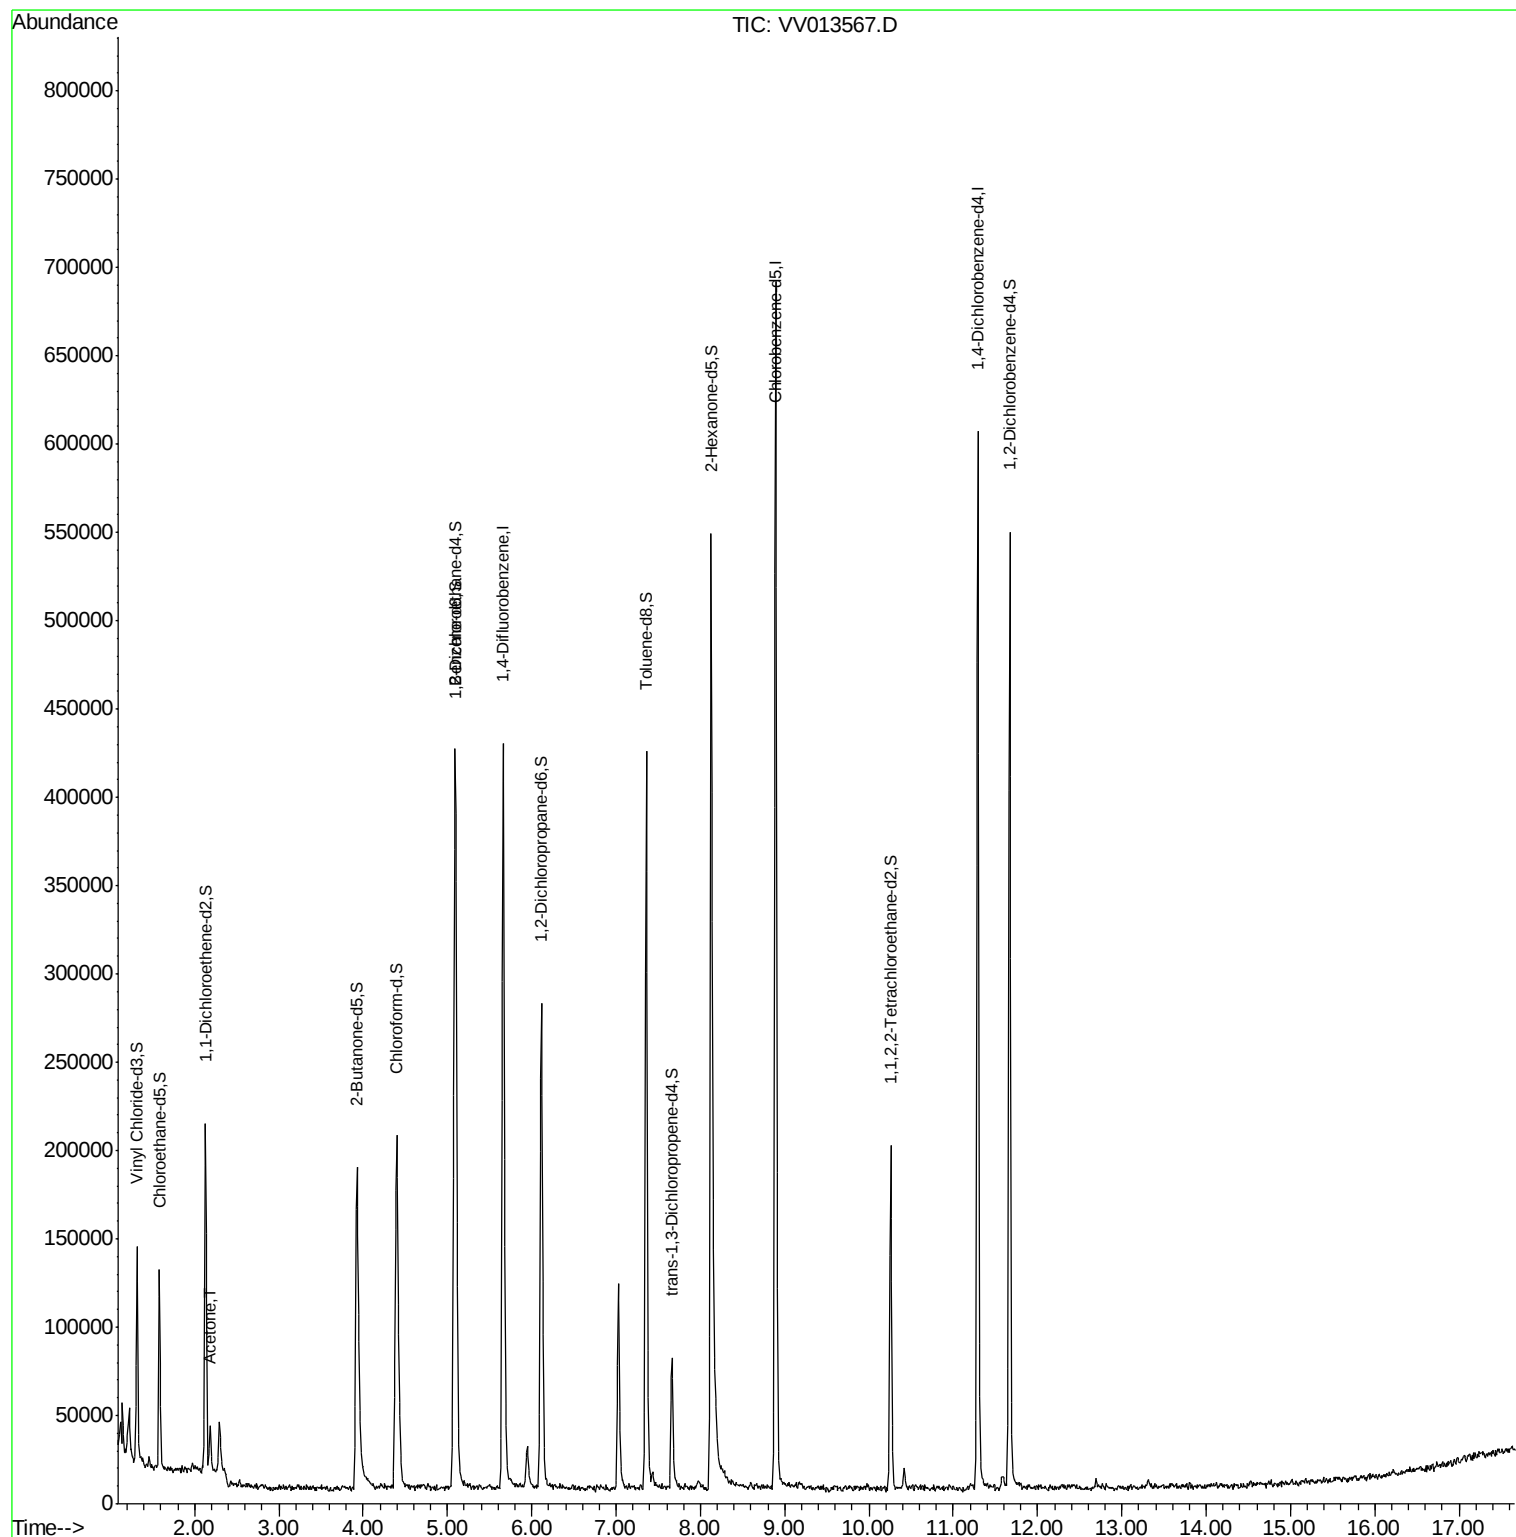

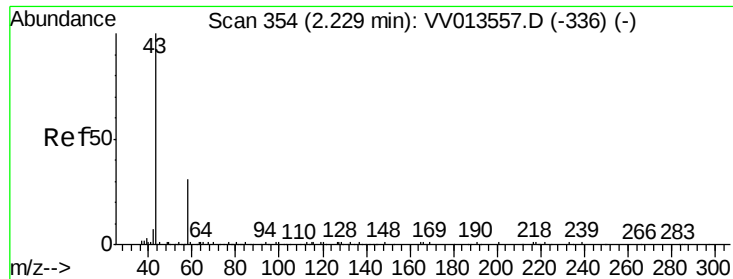

#13

Acetone

Concen: 6.985 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.04 min

Lab File: VV013567.D

Acq: 09 Nov 2019 03:21

Instrument :
MSVOA_V
ClientSampleId :
F2J12

Tot Ion: 43 Resp: 23377

Ion Ratio Lower Upper

43 100

58 34.3 0.0 60.8

