

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110819\
 Data File : VV013571.D
 Acq On : 09 Nov 2019 04:57
 Operator : SY/MD
 Sample : K5747-21
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2J17

Quant Time: Nov 11 00:33:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 11 00:28:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	371778	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	373993	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	164401	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	79645	5.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.60%
7) Chloroethane-d5	1.58	69	73997	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.40%
11) 1,1-Dichloroethene-d2	2.13	63	99253	3.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.00%
20) 2-Butanone-d5	3.92	46	290254	51.67	ug/L	-0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.34%
24) Chloroform-d	4.40	84	195276	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.08	65	113649	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.10	84	362271	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.11	67	130431	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.36	98	272748	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	7.66	79	41970	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.13	63	170814	43.40	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.80%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	93187	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	149406	5.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.00%


Target Compounds				Ovalue
13) Acetone	2.19	43	21574	6.331 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110819\
Data File : VV013571.D
Acq On : 09 Nov 2019 04:57
Operator : SY/MD
Sample : K5747-21
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2J17

Quant Time: Nov 11 00:33:55 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 11 00:28:08 2019
Response via : Initial Calibration

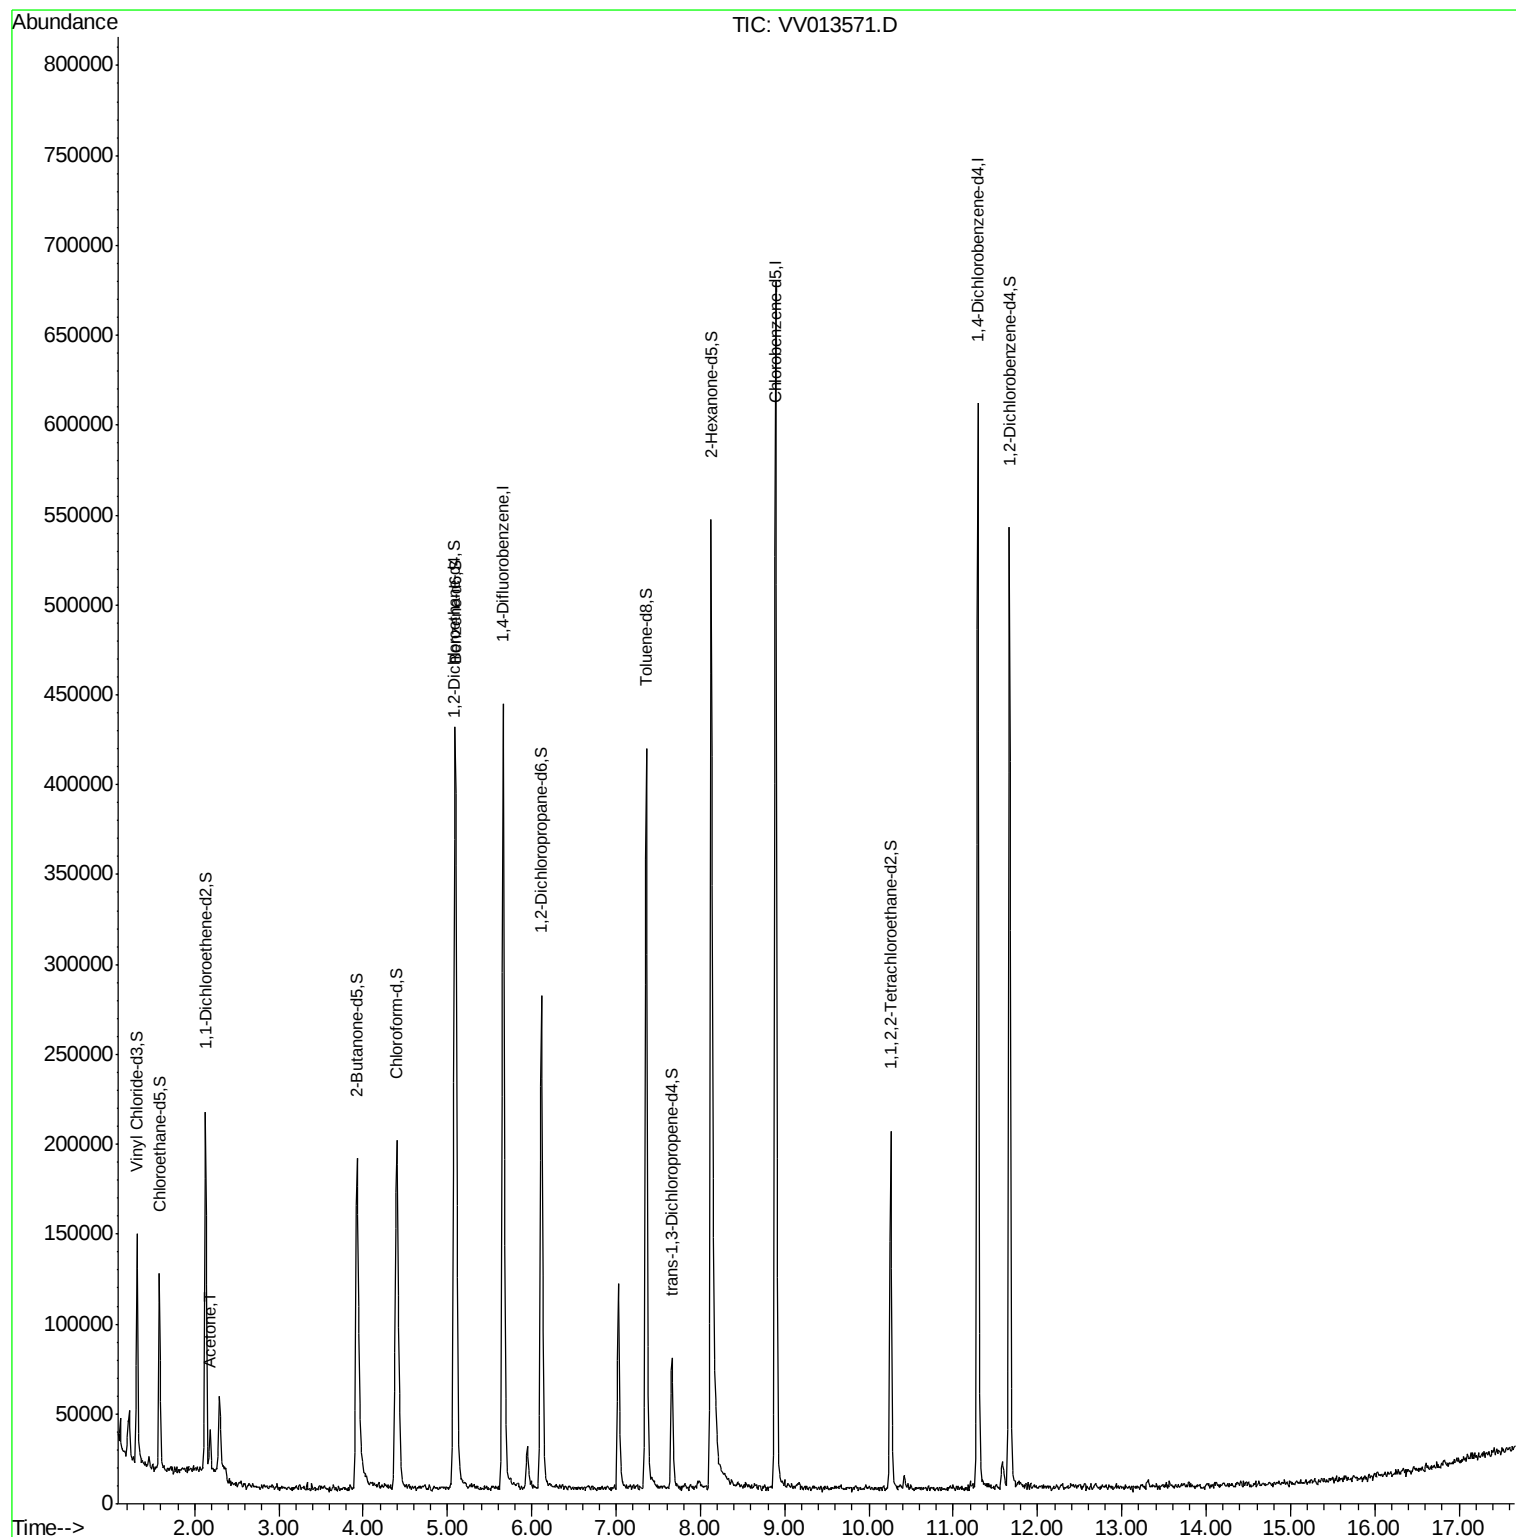

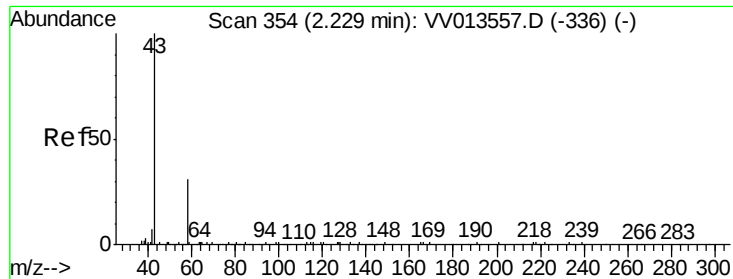

#13

Acetone

Concen: 6.331 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.04 min

Lab File: VV013571.D

Acq: 09 Nov 2019 04:57

Instrument :
MSVOA_V
ClientSampleId :
F2J17

Tot Ion: 43 Resp: 21574

Ion Ratio Lower Upper

43 100

58 34.1 0.0 60.8

