

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019292.D
 Acq On : 06 Nov 2020 12:35
 Operator : SY/MD
 Sample : L4615-17ME
 Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG485ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.219	36	40	47	rVB	11417	10133	0.15%	0.066%
2	1.312	63	69	86	rVB	119127	149941	2.24%	0.981%
3	1.547	136	142	145	rBV	24804	28842	0.43%	0.189%
4	1.573	146	150	163	rVB	86334	129585	1.94%	0.848%
5	2.097	303	313	325	rBV	250891	368440	5.51%	2.410%
6	2.367	393	397	398	rBV	329	217	0.00%	0.001%
7	2.511	437	442	451	rVB4	2235	2922	0.04%	0.019%
8	2.630	466	479	494	rBV2	9687	21598	0.32%	0.141%
9	2.952	578	579	583	rVB2	408	229	0.00%	0.001%
10	2.974	583	586	587	rBV	313	169	0.00%	0.001%
11	3.093	621	623	627	rVB	344	228	0.00%	0.001%
12	3.119	627	631	634	rBV2	296	320	0.00%	0.002%
13	3.164	642	645	647	rBV	222	150	0.00%	0.001%
14	3.312	689	691	693	rVB2	287	131	0.00%	0.001%
15	3.450	728	734	735	rBV	382	317	0.00%	0.002%
16	3.595	775	779	783	rBV	331	268	0.00%	0.002%
17	3.627	787	789	791	rBV2	181	84	0.00%	0.001%
18	3.666	797	801	805	rBV	242	293	0.00%	0.002%
19	3.698	810	811	812	rBV	140	44	0.00%	0.000%
20	3.714	812	816	818	rBV2	178	158	0.00%	0.001%
21	3.765	826	832	836	rBV	226	289	0.00%	0.002%
22	3.807	841	845	849	rBV	270	241	0.00%	0.002%
23	3.843	854	856	861	rVV2	213	179	0.00%	0.001%
24	3.917	869	879	915	rBV2	48751	190971	2.86%	1.249%
25	4.367	1004	1019	1047	rVB	166250	417456	6.24%	2.731%
26	4.601	1088	1092	1094	rVB	181	137	0.00%	0.001%
27	4.627	1097	1100	1103	rBV3	276	179	0.00%	0.001%
28	4.656	1106	1109	1112	rBV2	300	207	0.00%	0.001%
29	4.781	1143	1148	1149	rBV	253	202	0.00%	0.001%
30	4.855	1166	1171	1174	rBV2	431	414	0.01%	0.003%
31	4.904	1181	1186	1189	rBV2	245	279	0.00%	0.002%
32	4.942	1195	1198	1199	rBV2	222	153	0.00%	0.001%
33	5.061	1219	1235	1261	rBV2	428486	1058395	15.82%	6.923%
34	5.341	1319	1322	1324	rBV	890	603	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019292.D
 Acq On : 06 Nov 2020 12:35
 Operator : SY/MD
 Sample : L4615-17ME
 Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG485ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.547	1383	1386	1390	rVB2	437	301	0.00%	0.002%
36	5.566	1390	1392	1393	rBV	287	121	0.00%	0.001%
37	5.634	1400	1413	1441	rBV	315627	654637	9.79%	4.282%
38	5.929	1491	1505	1524	rBV3	146993	311219	4.65%	2.036%
39	6.087	1541	1554	1586	rVB	233282	488206	7.30%	3.193%
40	6.354	1634	1637	1638	rBV	109	65	0.00%	0.000%
41	6.428	1658	1660	1662	rBV	192	119	0.00%	0.001%
42	6.444	1663	1665	1669	rVV2	276	168	0.00%	0.001%
43	6.556	1696	1700	1703	rBV3	336	257	0.00%	0.002%
44	6.659	1729	1732	1737	rVB3	1028	780	0.01%	0.005%
45	6.688	1737	1741	1745	rVB4	550	558	0.01%	0.004%
46	6.714	1745	1749	1752	rBV4	414	326	0.00%	0.002%
47	6.794	1772	1774	1777	rVB	260	116	0.00%	0.001%
48	6.826	1781	1784	1786	rBV2	223	140	0.00%	0.001%
49	6.859	1792	1794	1795	rBV2	170	58	0.00%	0.000%
50	6.894	1801	1805	1810	rBV2	429	352	0.01%	0.002%
51	7.003	1825	1839	1875	rBV	129641	255777	3.82%	1.673%
52	7.212	1902	1904	1913	rVB4	895	939	0.01%	0.006%
53	7.244	1913	1914	1915	rBV4	300	107	0.00%	0.001%
54	7.286	1924	1927	1928	rBV	185	100	0.00%	0.001%
55	7.331	1929	1941	1961	rBV	472259	846911	12.66%	5.540%
56	7.547	2005	2008	2011	rBV3	410	308	0.00%	0.002%
57	7.640	2026	2037	2064	rBV	89810	178834	2.67%	1.170%
58	7.994	2130	2147	2175	rBV	3961579	6688135	100.00%	43.746%
59	8.135	2175	2191	2230	rVB3	155461	498141	7.45%	3.258%
60	8.556	2320	2322	2324	rBV	369	182	0.00%	0.001%
61	8.630	2342	2345	2348	rBV2	438	348	0.01%	0.002%
62	8.694	2363	2365	2366	rBV	246	119	0.00%	0.001%
63	8.797	2394	2397	2398	rBV	222	142	0.00%	0.001%
64	8.871	2409	2420	2449	rBV	464360	845390	12.64%	5.530%
65	9.228	2527	2531	2534	rBV2	487	393	0.01%	0.003%
66	9.331	2560	2563	2568	rBV	277	290	0.00%	0.002%
67	9.395	2579	2583	2587	rBV2	375	385	0.01%	0.003%
68	9.530	2621	2625	2628	rBV2	296	227	0.00%	0.001%
69	9.836	2718	2720	2723	rBV	270	118	0.00%	0.001%
70	10.074	2792	2794	2797	rBV	306	169	0.00%	0.001%
71	10.145	2810	2816	2820	rBV3	1483	1747	0.03%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019292.D
 Acq On : 06 Nov 2020 12:35
 Operator : SY/MD
 Sample : L4615-17ME
 Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG485ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.244	2830	2847	2864	rBV	273529	469213	7.02%	3.069%
73	10.502	2924	2927	2931	rVB2	291	229	0.00%	0.001%
74	10.521	2931	2933	2936	rBV2	200	118	0.00%	0.001%
75	10.547	2937	2941	2943	rVB2	236	154	0.00%	0.001%
76	10.563	2943	2946	2948	rBV2	319	191	0.00%	0.001%
77	10.624	2963	2965	2971	rVB3	425	274	0.00%	0.002%
78	10.884	3042	3046	3049	rBV2	358	294	0.00%	0.002%
79	10.939	3058	3063	3074	rVB5	1497	2354	0.04%	0.015%
80	11.058	3097	3100	3103	rBV2	358	295	0.00%	0.002%
81	11.135	3121	3124	3128	rBV2	269	251	0.00%	0.002%
82	11.167	3129	3134	3138	rVV3	700	778	0.01%	0.005%
83	11.273	3155	3167	3197	rBV	532547	827532	12.37%	5.413%
84	11.511	3237	3241	3244	rBV3	472	371	0.01%	0.002%
85	11.582	3259	3263	3266	rBV	360	386	0.01%	0.003%
86	11.649	3271	3284	3302	rBV	528325	822846	12.30%	5.382%
87	11.807	3331	3333	3337	rBV2	403	326	0.00%	0.002%
88	12.035	3402	3404	3412	rBV	292	301	0.00%	0.002%
89	12.077	3412	3417	3420	rBV2	345	348	0.01%	0.002%
90	12.251	3467	3471	3472	rBV2	345	240	0.00%	0.002%
91	12.276	3472	3479	3486	rVB4	1335	1950	0.03%	0.013%
92	12.839	3652	3654	3656	rBV2	241	167	0.00%	0.001%


Sum of corrected areas: 15288577

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110820\
Data File : VV019292.D
Acq On : 06 Nov 2020 12:35
Operator : SY/MD
Sample : L4615-17ME
Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG485ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

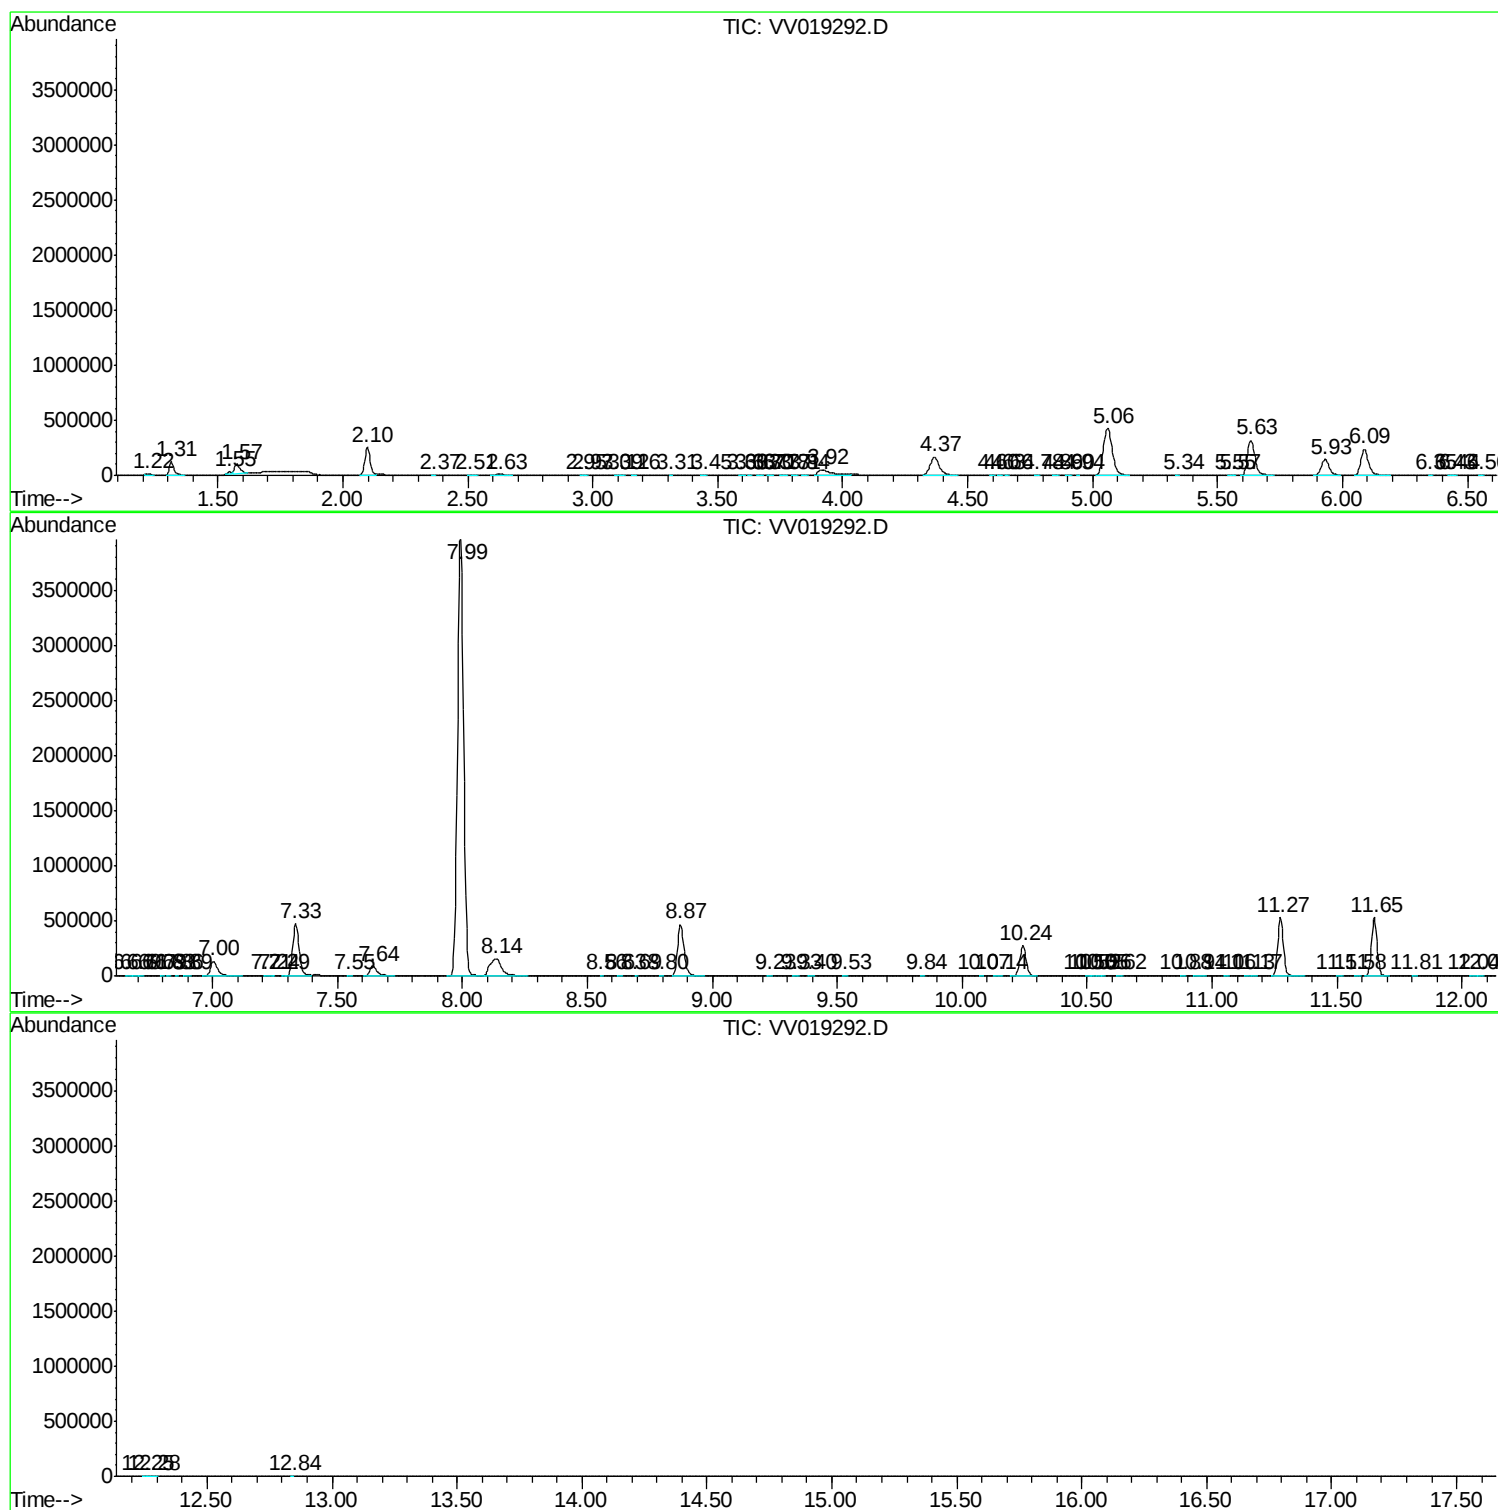

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110820\
Data File : VV019292.D
Acq On : 06 Nov 2020 12:35
Operator : SY/MD
Sample : L4615-17ME
Misc : 5.76g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG485ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110820\
Data File : VV019292.D
Acq On : 06 Nov 2020 12:35
Operator : SY/MD
Sample : L4615-17ME
Misc : 5.76g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG485ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc