

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019295.D
 Acq On : 06 Nov 2020 14:11
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	144266	144594	14.25%	1.827%
2	1.579	144	152	164	rBV	118121	135077	13.32%	1.706%
3	2.122	311	321	347	rVB	240250	365192	36.00%	4.614%
4	2.306	374	378	380	rBV2	527	344	0.03%	0.004%
5	2.393	404	405	412	rVB2	309	298	0.03%	0.004%
6	2.454	418	424	427	rBV3	396	387	0.04%	0.005%
7	2.569	456	460	462	rBV2	428	271	0.03%	0.003%
8	2.730	508	510	513	rBV	184	99	0.01%	0.001%
9	2.753	513	517	519	rBV2	199	167	0.02%	0.002%
10	2.782	521	526	529	rBV2	304	287	0.03%	0.004%
11	2.875	551	555	560	rVB2	272	243	0.02%	0.003%
12	2.910	560	566	567	rBV	254	244	0.02%	0.003%
13	3.200	654	656	659	rBV2	171	116	0.01%	0.001%
14	3.277	677	680	681	rBV	185	102	0.01%	0.001%
15	3.296	683	686	691	rVB2	370	307	0.03%	0.004%
16	3.325	691	695	698	rBV2	291	253	0.02%	0.003%
17	3.441	728	731	734	rVB2	347	162	0.02%	0.002%
18	3.685	801	807	812	rBV2	394	566	0.06%	0.007%
19	3.843	852	856	859	rVB2	301	235	0.02%	0.003%
20	3.859	859	861	863	rBV	156	51	0.01%	0.001%
21	3.910	863	877	917	rBV	68762	221373	21.82%	2.797%
22	4.373	1006	1021	1055	rVB	165355	408438	40.26%	5.160%
23	4.576	1082	1084	1090	rVB3	433	327	0.03%	0.004%
24	4.730	1129	1132	1134	rBV	394	281	0.03%	0.004%
25	4.820	1157	1160	1164	rVB2	329	194	0.02%	0.002%
26	4.839	1164	1166	1172	rBV	125	133	0.01%	0.002%
27	4.865	1172	1174	1176	rBV2	315	185	0.02%	0.002%
28	5.068	1218	1237	1274	rBV2	391594	1014435	100.00%	12.816%
29	5.293	1304	1307	1308	rBV	306	161	0.02%	0.002%
30	5.380	1332	1334	1335	rBV	168	81	0.01%	0.001%
31	5.421	1346	1347	1349	rBV	167	87	0.01%	0.001%
32	5.454	1354	1357	1360	rVB2	420	254	0.03%	0.003%
33	5.470	1360	1362	1364	rBV2	219	137	0.01%	0.002%
34	5.540	1382	1384	1388	rBV2	253	179	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019295.D
 Acq On : 06 Nov 2020 14:11
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.637	1401	1414	1438	rBV	320702	641297	63.22%	8.102%
36	5.926	1494	1504	1523	rVV3	18780	37257	3.67%	0.471%
37	5.994	1523	1525	1528	rVB	630	370	0.04%	0.005%
38	6.013	1528	1531	1534	rBV	216	187	0.02%	0.002%
39	6.090	1542	1555	1580	rBV	230301	466124	45.95%	5.889%
40	6.338	1629	1632	1634	rBV	269	196	0.02%	0.002%
41	6.367	1639	1641	1642	rBV	176	57	0.01%	0.001%
42	6.656	1728	1731	1732	rBV2	279	166	0.02%	0.002%
43	6.817	1778	1781	1782	rBV	202	122	0.01%	0.002%
44	7.003	1829	1839	1860	rBV	129321	234548	23.12%	2.963%
45	7.334	1930	1942	1961	rBV	455963	785649	77.45%	9.925%
46	7.640	2027	2037	2065	rBV	93889	163557	16.12%	2.066%
47	7.994	2144	2147	2156	rVB5	1265	1731	0.17%	0.022%
48	8.035	2156	2160	2162	rBV	229	207	0.02%	0.003%
49	8.106	2172	2182	2219	rBV2	233967	447698	44.13%	5.656%
50	8.505	2304	2306	2307	rBV	194	67	0.01%	0.001%
51	8.659	2352	2354	2357	rBV	281	179	0.02%	0.002%
52	8.733	2376	2377	2378	rBV	210	68	0.01%	0.001%
53	8.871	2405	2420	2447	rBV	503408	815417	80.38%	10.301%
54	9.141	2502	2504	2506	rBV	224	137	0.01%	0.002%
55	9.161	2508	2510	2512	rBV2	390	242	0.02%	0.003%
56	9.360	2567	2572	2574	rBV	224	203	0.02%	0.003%
57	9.543	2626	2629	2630	rBV	163	92	0.01%	0.001%
58	9.604	2646	2648	2651	rVB2	134	78	0.01%	0.001%
59	9.630	2652	2656	2660	rBV2	294	290	0.03%	0.004%
60	9.701	2673	2678	2684	rBV2	354	456	0.04%	0.006%
61	9.736	2688	2689	2692	rVB	186	93	0.01%	0.001%
62	9.752	2692	2694	2696	rBV	175	101	0.01%	0.001%
63	9.820	2711	2715	2717	rBV2	368	304	0.03%	0.004%
64	9.971	2760	2762	2765	rBV	124	73	0.01%	0.001%
65	10.145	2812	2816	2820	rBV2	1013	807	0.08%	0.010%
66	10.235	2829	2844	2863	rBV	277989	438860	43.26%	5.544%
67	10.434	2903	2906	2910	rBV	310	235	0.02%	0.003%
68	10.495	2921	2925	2928	rBV	344	316	0.03%	0.004%
69	10.701	2985	2989	2992	rBV	356	330	0.03%	0.004%
70	10.897	3047	3050	3051	rBV	264	155	0.02%	0.002%
71	10.932	3056	3061	3068	rVV3	833	1249	0.12%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019295.D
 Acq On : 06 Nov 2020 14:11
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	11.000	3076	3082	3084	rBV2	356	374	0.04%	0.005%
73	11.100	3111	3113	3115	rBV	329	189	0.02%	0.002%
74	11.161	3130	3132	3133	rBV	238	84	0.01%	0.001%
75	11.199	3141	3144	3147	rBV2	315	225	0.02%	0.003%
76	11.270	3154	3166	3188	rBV	515264	793730	78.24%	10.027%
77	11.646	3270	3283	3302	rBV	500285	784859	77.37%	9.915%
78	11.791	3323	3328	3330	rBV2	627	535	0.05%	0.007%
79	12.083	3417	3419	3420	rBV2	127	67	0.01%	0.001%
80	12.360	3503	3505	3506	rBV	222	94	0.01%	0.001%
81	13.273	3787	3789	3792	rBV	344	213	0.02%	0.003%
82	13.543	3870	3873	3876	rBV	506	393	0.04%	0.005%
83	14.334	4113	4119	4120	rBV2	622	640	0.06%	0.008%


Sum of corrected areas: 7915581

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110820\
Data File : VV019295.D
Acq On : 06 Nov 2020 14:11
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

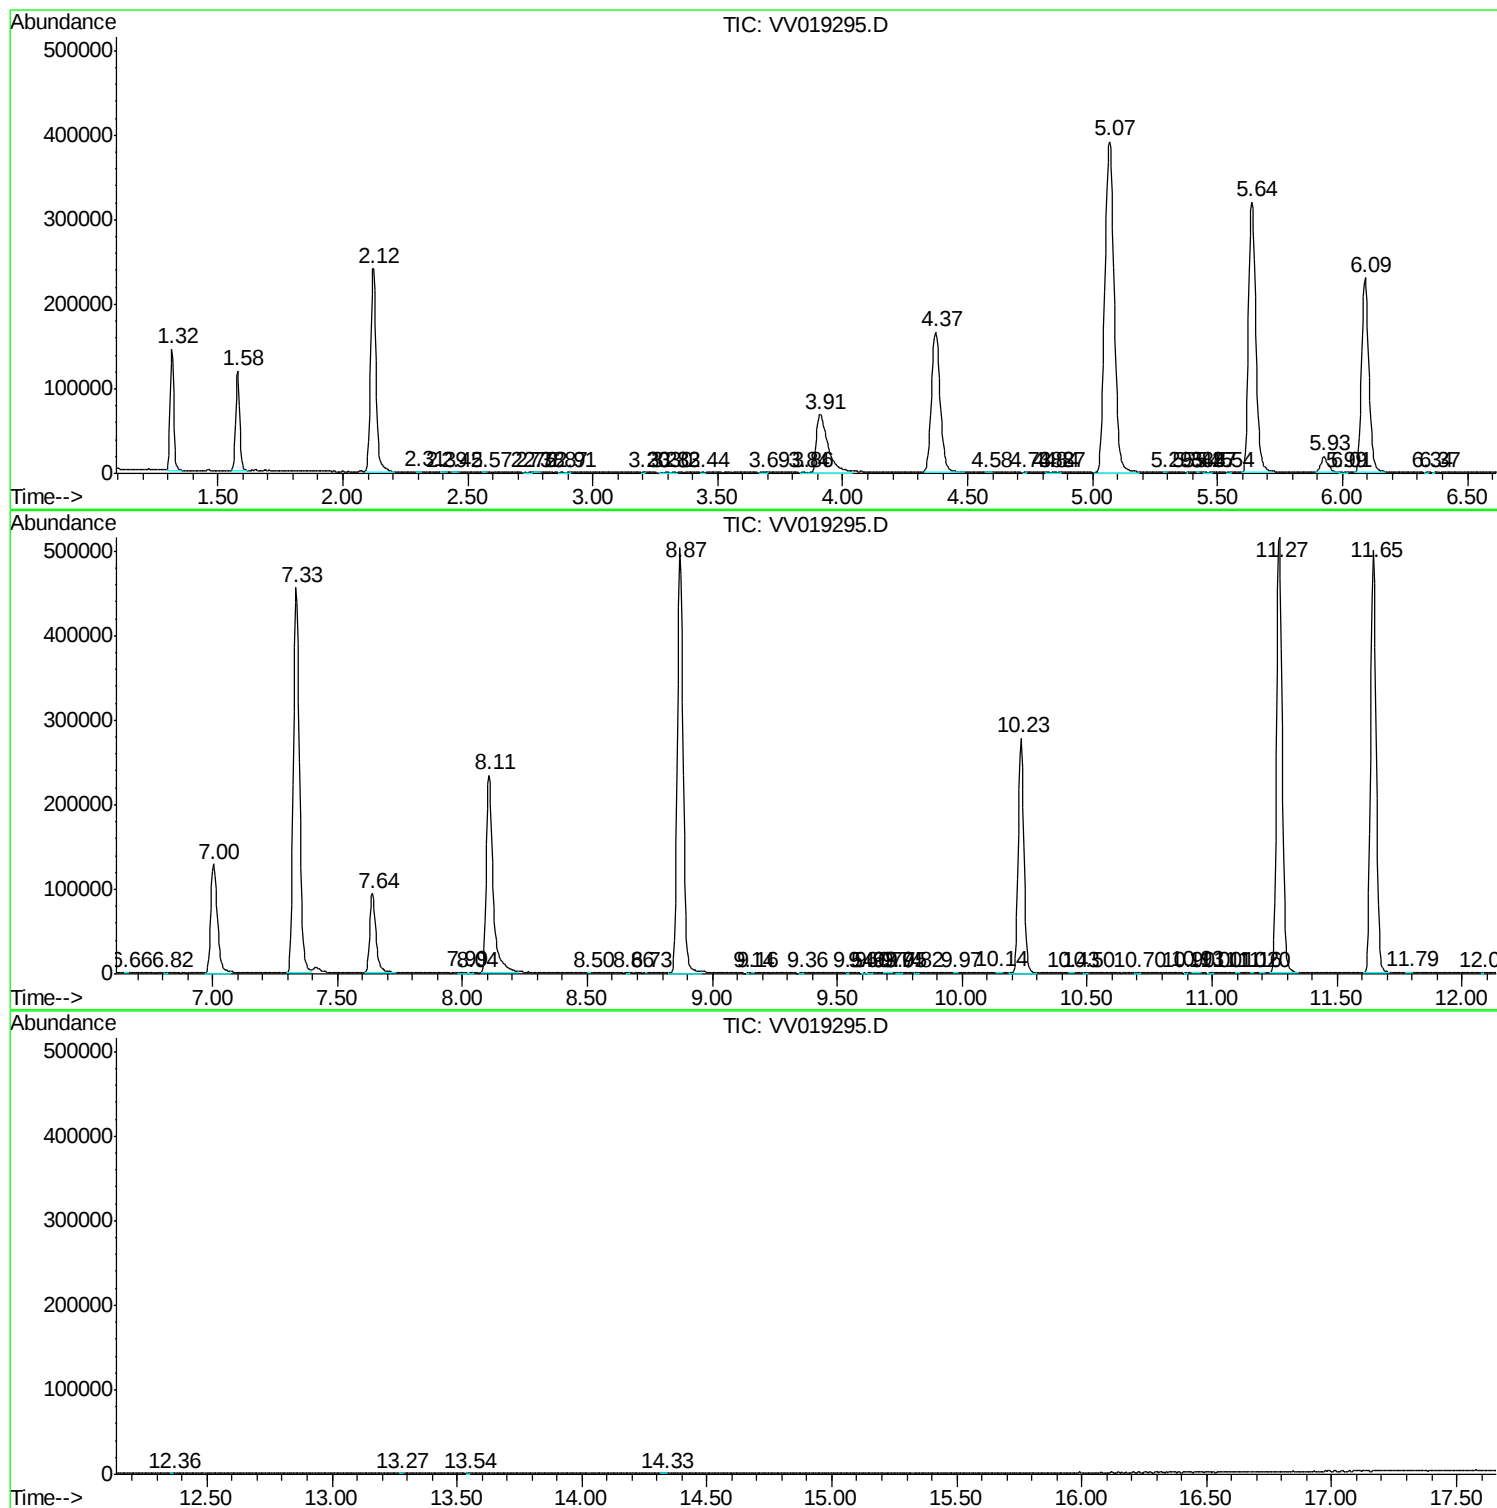

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110820\
Data File : VV019295.D
Acq On : 06 Nov 2020 14:11
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110820\
Data File : VV019295.D
Acq On : 06 Nov 2020 14:11
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc