

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019296.D
 Acq On : 06 Nov 2020 14:35
 Operator : SY/MD
 Sample : L4615-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG467

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	136895	138113	14.07%	1.805%
2	1.579	145	152	171	rVB	121979	136855	13.94%	1.788%
3	2.123	311	321	339	rBV	231657	345035	35.15%	4.508%
4	2.389	402	404	407	rBV	251	130	0.01%	0.002%
5	2.592	464	467	470	rBV	265	134	0.01%	0.002%
6	2.714	500	505	506	rBV	331	252	0.03%	0.003%
7	2.778	518	525	536	rVB4	1389	2690	0.27%	0.035%
8	2.926	565	571	575	rBV2	270	367	0.04%	0.005%
9	3.061	603	613	628	rVB4	7730	16298	1.66%	0.213%
10	3.171	643	647	651	rBV2	263	320	0.03%	0.004%
11	3.209	656	659	662	rVB2	280	203	0.02%	0.003%
12	3.270	675	678	683	rVB2	189	154	0.02%	0.002%
13	3.303	687	688	690	rVB2	110	31	0.00%	0.000%
14	3.319	690	693	695	rBV	256	188	0.02%	0.002%
15	3.377	709	711	713	rBV2	121	69	0.01%	0.001%
16	3.415	719	723	731	rVB2	326	536	0.05%	0.007%
17	3.450	731	734	736	rBV	218	138	0.01%	0.002%
18	3.515	752	754	759	rBV2	187	123	0.01%	0.002%
19	3.589	763	777	784	rBV2	470	1120	0.11%	0.015%
20	3.621	784	787	788	rBV2	127	74	0.01%	0.001%
21	3.631	788	790	796	rVB2	304	239	0.02%	0.003%
22	3.659	796	799	802	rBV	249	142	0.01%	0.002%
23	3.788	828	839	856	rVB4	6201	14733	1.50%	0.193%
24	3.859	856	861	864	rVB	295	248	0.03%	0.003%
25	3.913	868	878	907	rBV	67137	205293	20.91%	2.682%
26	4.376	1006	1022	1050	rBV	161240	397282	40.47%	5.191%
27	4.630	1099	1101	1103	rBV	328	184	0.02%	0.002%
28	4.682	1115	1117	1120	rBV3	242	116	0.01%	0.002%
29	4.756	1138	1140	1143	rBV2	233	119	0.01%	0.002%
30	4.775	1145	1146	1148	rBV	147	72	0.01%	0.001%
31	4.843	1164	1167	1168	rBV	239	120	0.01%	0.002%
32	5.071	1220	1238	1269	rBV2	379453	981671	100.00%	12.827%
33	5.373	1330	1332	1333	rBV2	324	107	0.01%	0.001%
34	5.409	1340	1343	1346	rBV	258	224	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019296.D
 Acq On : 06 Nov 2020 14:35
 Operator : SY/MD
 Sample : L4615-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG467

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.521	1376	1378	1379	rBV	216	69	0.01%	0.001%
36	5.585	1395	1398	1403	rVB2	361	306	0.03%	0.004%
37	5.640	1403	1415	1442	rBV	305084	606150	61.75%	7.920%
38	5.820	1470	1471	1472	rBV	245	88	0.01%	0.001%
39	5.865	1482	1485	1489	rBV	262	201	0.02%	0.003%
40	5.929	1495	1505	1525	rVV2	20584	41671	4.24%	0.544%
41	6.013	1529	1531	1532	rVB2	141	32	0.00%	0.000%
42	6.093	1543	1556	1585	rBV	222210	451765	46.02%	5.903%
43	6.319	1624	1626	1628	rBV	311	178	0.02%	0.002%
44	6.335	1628	1631	1635	rVV2	383	325	0.03%	0.004%
45	6.460	1667	1670	1676	rBV2	300	378	0.04%	0.005%
46	6.521	1687	1689	1691	rBV	127	59	0.01%	0.001%
47	6.585	1706	1709	1712	rVB2	475	278	0.03%	0.004%
48	6.598	1712	1713	1715	rVB2	273	54	0.01%	0.001%
49	6.627	1719	1722	1725	rBV2	222	154	0.02%	0.002%
50	6.653	1728	1730	1731	rBV	301	134	0.01%	0.002%
51	6.733	1753	1755	1757	rVV	300	99	0.01%	0.001%
52	6.746	1757	1759	1763	rVB	180	67	0.01%	0.001%
53	7.007	1828	1840	1863	rBV2	125990	227714	23.20%	2.975%
54	7.283	1923	1926	1931	rBV2	441	468	0.05%	0.006%
55	7.338	1931	1943	1960	rBV	444246	762152	77.64%	9.959%
56	7.640	2028	2037	2071	rBV2	87368	158065	16.10%	2.065%
57	7.791	2081	2084	2087	rBV4	442	329	0.03%	0.004%
58	7.958	2125	2136	2145	rBV4	3440	6191	0.63%	0.081%
59	8.106	2172	2182	2223	rBV	233086	456262	46.48%	5.962%
60	8.511	2303	2308	2312	rVB	443	508	0.05%	0.007%
61	8.531	2312	2314	2315	rBV	212	91	0.01%	0.001%
62	8.579	2325	2329	2331	rBV	378	285	0.03%	0.004%
63	8.675	2355	2359	2363	rBV2	442	467	0.05%	0.006%
64	8.772	2385	2389	2391	rBV2	280	252	0.03%	0.003%
65	8.798	2394	2397	2399	rBV	272	205	0.02%	0.003%
66	8.871	2409	2420	2452	rBV	472933	762292	77.65%	9.960%
67	9.347	2565	2568	2574	rBV2	249	246	0.03%	0.003%
68	9.508	2615	2618	2621	rBV2	338	332	0.03%	0.004%
69	9.627	2652	2655	2662	rBV	304	295	0.03%	0.004%
70	9.836	2718	2720	2723	rBV	334	236	0.02%	0.003%
71	10.074	2790	2794	2796	rBV	258	196	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019296.D
 Acq On : 06 Nov 2020 14:35
 Operator : SY/MD
 Sample : L4615-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG467

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.235	2832	2844	2870	rVB	267662	419122	42.69%	5.476%
73	10.325	2870	2872	2873	rBV	343	156	0.02%	0.002%
74	10.402	2886	2896	2907	rBV3	7631	12226	1.25%	0.160%
75	10.453	2910	2912	2914	rBV	183	80	0.01%	0.001%
76	10.965	3056	3071	3080	rBV8	2068	5193	0.53%	0.068%
77	11.113	3113	3117	3119	rBV2	219	179	0.02%	0.002%
78	11.206	3143	3146	3149	rVB	324	172	0.02%	0.002%
79	11.270	3155	3166	3190	rBV	478663	736341	75.01%	9.621%
80	11.646	3271	3283	3300	rBV	489028	755377	76.95%	9.870%
81	11.871	3350	3353	3354	rBV2	403	169	0.02%	0.002%
82	12.212	3456	3459	3461	rBV	272	213	0.02%	0.003%
83	12.350	3498	3502	3505	rBV2	282	282	0.03%	0.004%
84	12.765	3627	3631	3633	rBV2	303	231	0.02%	0.003%
85	12.778	3633	3635	3637	rBV	316	144	0.01%	0.002%
86	12.952	3686	3689	3691	rBV	298	204	0.02%	0.003%
87	13.170	3754	3757	3759	rBV2	217	167	0.02%	0.002%
88	13.196	3762	3765	3768	rBV	307	224	0.02%	0.003%
89	13.858	3968	3971	3974	rBV2	326	282	0.03%	0.004%
90	14.128	4051	4055	4058	rBV	589	503	0.05%	0.007%


Sum of corrected areas: 7653239

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110820\
Data File : VV019296.D
Acq On : 06 Nov 2020 14:35
Operator : SY/MD
Sample : L4615-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG467

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

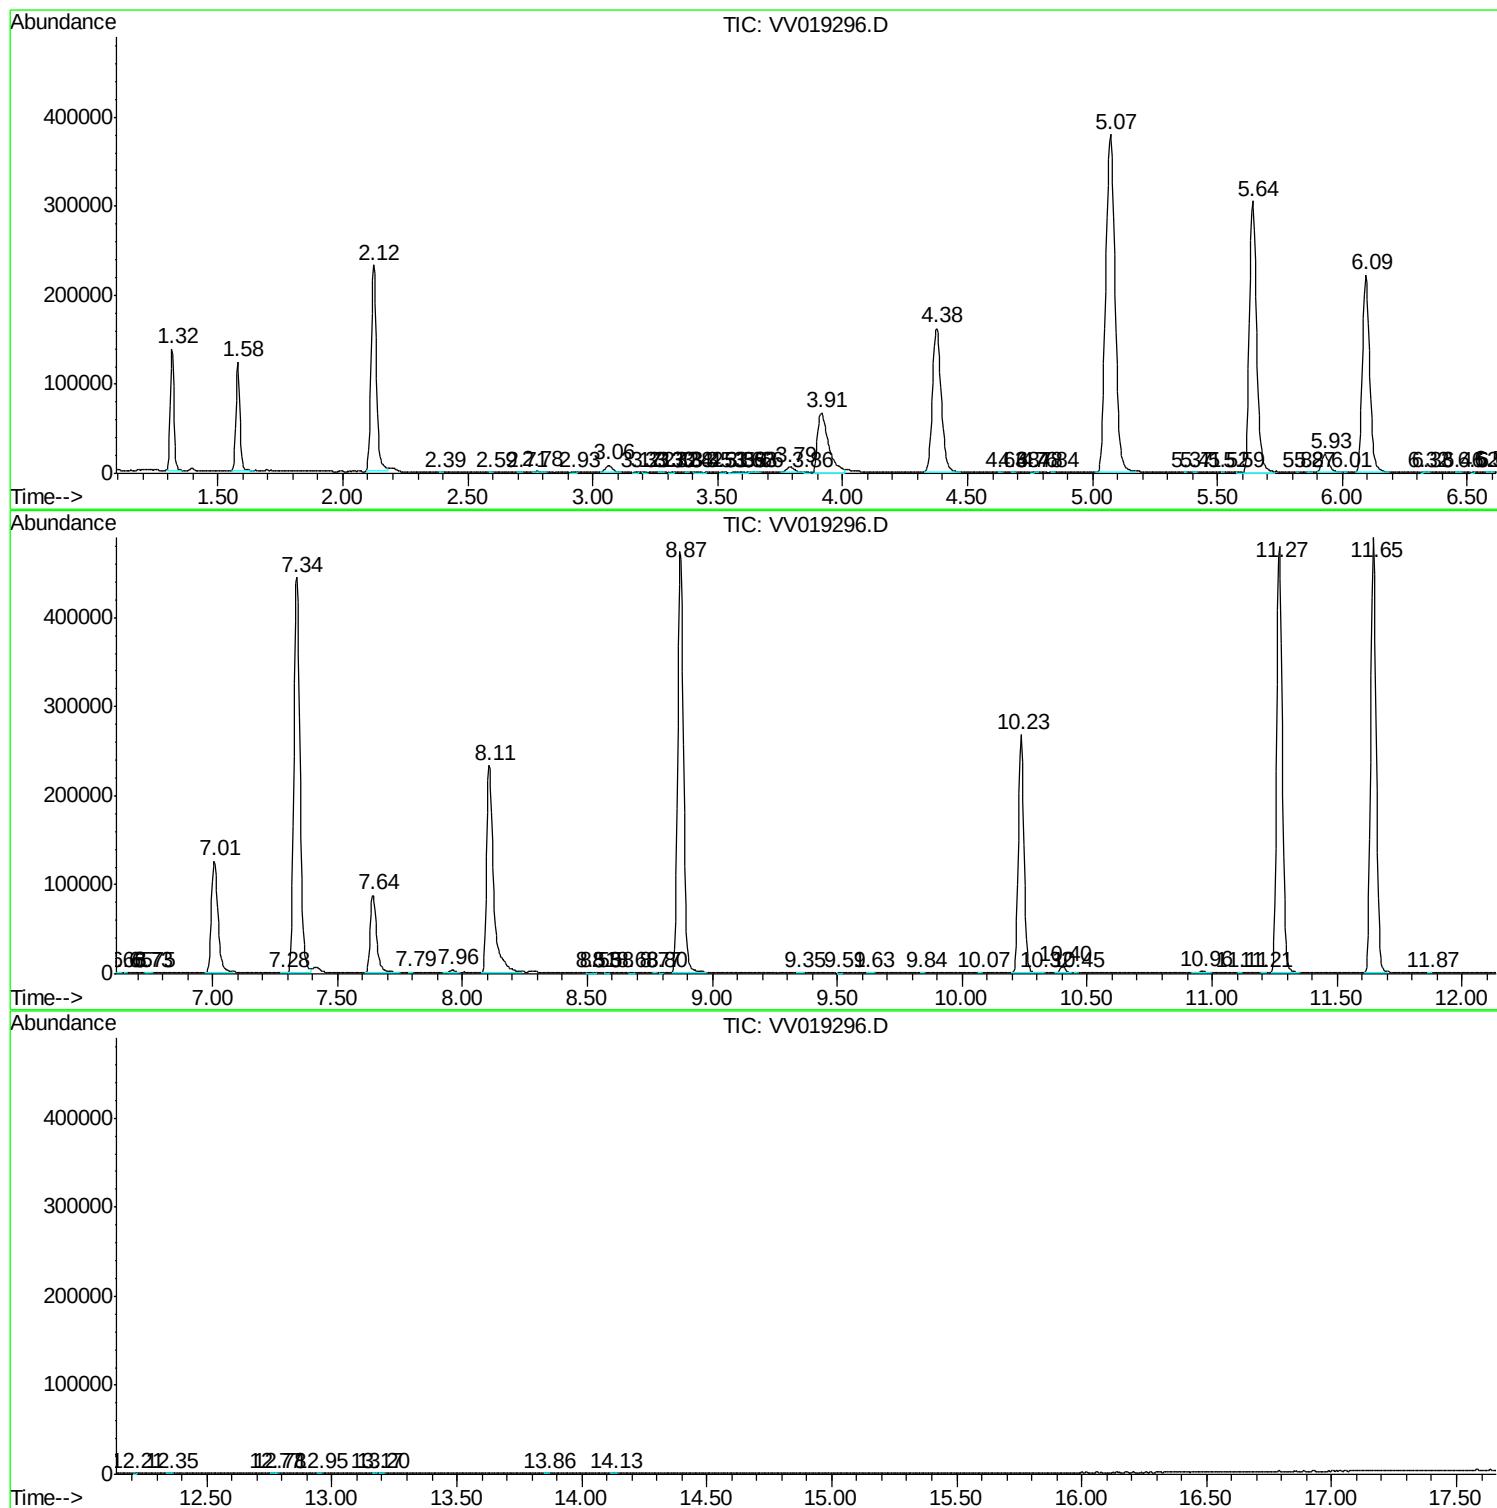

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110820\
Data File : VV019296.D
Acq On : 06 Nov 2020 14:35
Operator : SY/MD
Sample : L4615-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG467

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110820\
Data File : VV019296.D
Acq On : 06 Nov 2020 14:35
Operator : SY/MD
Sample : L4615-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG467

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc