

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019298.D
 Acq On : 06 Nov 2020 15:53
 Operator : SY/MD
 Sample : L4615-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	180843	181461	13.82%	1.966%
2	1.579	144	152	164	rBV	157812	177425	13.51%	1.922%
3	2.119	310	320	346	rVB	301917	460674	35.09%	4.991%
4	2.389	403	404	406	rBV	192	82	0.01%	0.001%
5	2.434	415	418	420	rBV2	398	259	0.02%	0.003%
6	2.524	439	446	455	rVB4	1561	2257	0.17%	0.024%
7	2.589	463	466	468	rBV2	263	155	0.01%	0.002%
8	2.772	520	523	525	rBV2	291	221	0.02%	0.002%
9	2.798	529	531	533	rBV2	275	131	0.01%	0.001%
10	2.827	537	540	542	rBV2	229	153	0.01%	0.002%
11	2.904	559	564	567	rBV	243	256	0.02%	0.003%
12	3.013	596	598	600	rBV	192	87	0.01%	0.001%
13	3.190	650	653	655	rBV2	352	226	0.02%	0.002%
14	3.228	663	665	666	rBV2	121	50	0.00%	0.001%
15	3.277	675	680	682	rBV	223	155	0.01%	0.002%
16	3.296	682	686	689	rBV2	291	205	0.02%	0.002%
17	3.444	727	732	734	rBV2	300	221	0.02%	0.002%
18	3.463	734	738	741	rBV2	193	162	0.01%	0.002%
19	3.508	750	752	754	rBV	115	44	0.00%	0.000%
20	3.563	762	769	772	rBV2	313	318	0.02%	0.003%
21	3.685	804	807	811	rBV	308	222	0.02%	0.002%
22	3.714	811	816	823	rBV2	362	515	0.04%	0.006%
23	3.762	827	831	833	rBV	240	183	0.01%	0.002%
24	3.814	841	847	851	rBV2	302	365	0.03%	0.004%
25	3.859	857	861	863	rBV	180	159	0.01%	0.002%
26	3.910	865	877	924	rVV2	91010	294955	22.47%	3.195%
27	4.370	1004	1020	1045	rBV	216229	527945	40.21%	5.719%
28	4.595	1087	1090	1091	rBV2	475	231	0.02%	0.003%
29	4.733	1129	1133	1135	rBV	273	201	0.02%	0.002%
30	4.971	1203	1207	1209	rBV	326	303	0.02%	0.003%
31	5.068	1218	1237	1265	rBV2	510035	1312934	100.00%	14.223%
32	5.412	1339	1344	1345	rBV3	455	311	0.02%	0.003%
33	5.502	1370	1372	1375	rBV2	405	253	0.02%	0.003%
34	5.566	1388	1392	1394	rBV	193	160	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019298.D
 Acq On : 06 Nov 2020 15:53
 Operator : SY/MD
 Sample : L4615-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.637	1402	1414	1442	rBV	264601	529906	40.36%	5.741%
36	5.926	1493	1504	1526	rVB3	19851	41895	3.19%	0.454%
37	6.035	1535	1538	1541	rBV2	526	386	0.03%	0.004%
38	6.090	1541	1555	1581	rVV	296380	604359	46.03%	6.547%
39	6.309	1621	1623	1627	rVB2	199	105	0.01%	0.001%
40	6.338	1627	1632	1637	rBV	205	304	0.02%	0.003%
41	6.363	1638	1640	1644	rVV	314	170	0.01%	0.002%
42	6.402	1649	1652	1654	rBV	300	175	0.01%	0.002%
43	6.418	1654	1657	1660	rVV2	299	187	0.01%	0.002%
44	6.505	1682	1684	1686	rBV	136	54	0.00%	0.001%
45	6.595	1710	1712	1715	rBV2	236	176	0.01%	0.002%
46	6.646	1725	1728	1731	rBV2	287	254	0.02%	0.003%
47	6.672	1731	1736	1738	rVV2	529	484	0.04%	0.005%
48	6.711	1746	1748	1751	rBV	235	159	0.01%	0.002%
49	6.749	1758	1760	1761	rBV	231	85	0.01%	0.001%
50	6.778	1767	1769	1772	rBV2	304	200	0.02%	0.002%
51	6.846	1788	1790	1793	rBV2	271	160	0.01%	0.002%
52	6.913	1808	1811	1816	rBV	277	258	0.02%	0.003%
53	7.003	1828	1839	1859	rBV	171038	307364	23.41%	3.330%
54	7.334	1930	1942	1960	rBV	600849	1028037	78.30%	11.137%
55	7.640	2026	2037	2058	rBV	121138	213386	16.25%	2.312%
56	7.842	2097	2100	2102	rBV3	260	165	0.01%	0.002%
57	7.997	2145	2148	2157	rVB3	573	642	0.05%	0.007%
58	8.103	2171	2181	2220	rBV	323394	600633	45.75%	6.507%
59	8.457	2289	2291	2293	rBV2	244	142	0.01%	0.002%
60	8.485	2298	2300	2302	rBV	240	152	0.01%	0.002%
61	8.563	2316	2324	2329	rBV2	432	693	0.05%	0.008%
62	8.617	2338	2341	2344	rBV	301	202	0.02%	0.002%
63	8.688	2359	2363	2364	rBV2	251	140	0.01%	0.002%
64	8.746	2378	2381	2384	rBV2	295	213	0.02%	0.002%
65	8.804	2396	2399	2403	rBV2	256	214	0.02%	0.002%
66	8.871	2408	2420	2444	rBV	415116	669341	50.98%	7.251%
67	9.035	2468	2471	2473	rBV	486	312	0.02%	0.003%
68	9.257	2536	2540	2541	rBV	227	169	0.01%	0.002%
69	9.293	2548	2551	2552	rBV2	176	75	0.01%	0.001%
70	9.334	2560	2564	2565	rBV	238	139	0.01%	0.002%
71	9.354	2565	2570	2573	rVV2	156	186	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110820\
 Data File : VV019298.D
 Acq On : 06 Nov 2020 15:53
 Operator : SY/MD
 Sample : L4615-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.460	2599	2603	2607	rBV	413	368	0.03%	0.004%
73	9.498	2612	2615	2621	rVB2	435	388	0.03%	0.004%
74	9.534	2621	2626	2632	rBV2	365	540	0.04%	0.006%
75	9.682	2669	2672	2675	rBV	256	200	0.02%	0.002%
76	9.768	2693	2699	2703	rBV	490	670	0.05%	0.007%
77	9.839	2718	2721	2722	rBV	174	109	0.01%	0.001%
78	9.971	2756	2762	2769	rBV2	377	699	0.05%	0.008%
79	10.051	2784	2787	2793	rVB2	281	231	0.02%	0.003%
80	10.141	2810	2815	2823	rBV5	1663	2290	0.17%	0.025%
81	10.177	2823	2826	2828	rBV2	187	131	0.01%	0.001%
82	10.235	2832	2844	2863	rVV	374266	581053	44.26%	6.295%
83	10.620	2962	2964	2966	rBV2	286	150	0.01%	0.002%
84	10.714	2990	2993	2995	rBV	285	225	0.02%	0.002%
85	10.939	3057	3063	3073	rVB4	1326	1575	0.12%	0.017%
86	11.270	3154	3166	3190	rBV	430287	657334	50.07%	7.121%
87	11.646	3270	3283	3301	rBV	653888	1019634	77.66%	11.046%
88	12.505	3547	3550	3554	rBV2	271	304	0.02%	0.003%
89	13.617	3893	3896	3898	rBV	310	249	0.02%	0.003%


Sum of corrected areas: 9230951

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110820\
Data File : VV019298.D
Acq On : 06 Nov 2020 15:53
Operator : SY/MD
Sample : L4615-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

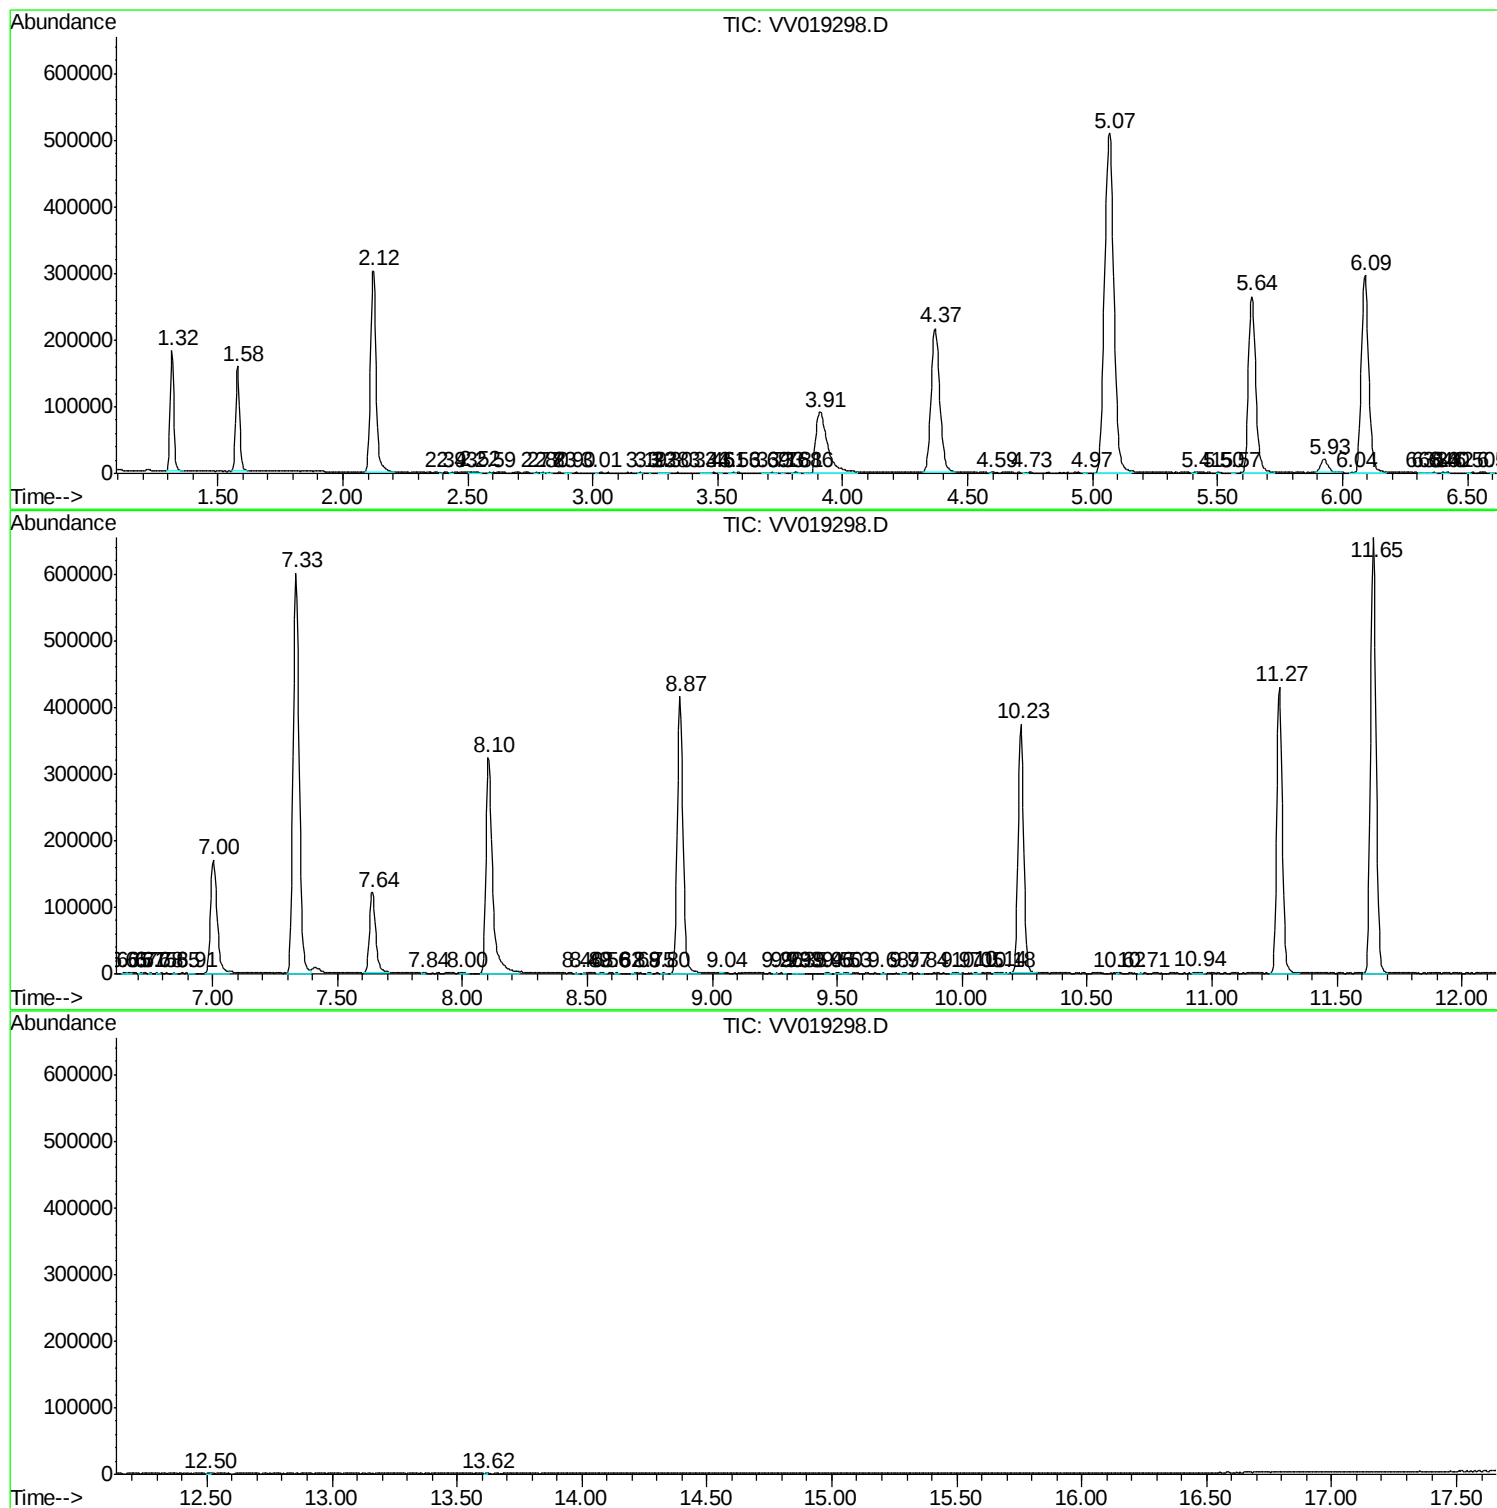

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110820\
Data File : VV019298.D
Acq On : 06 Nov 2020 15:53
Operator : SY/MD
Sample : L4615-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110820\
Data File : VV019298.D
Acq On : 06 Nov 2020 15:53
Operator : SY/MD
Sample : L4615-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc