


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV110820\
 Data File : VV019288.D
 Acq On : 06 Nov 2020 09:12
 Operator : SY/MD
 Sample : BFB90
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB90

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Mon Nov 09 02:16:03 2020

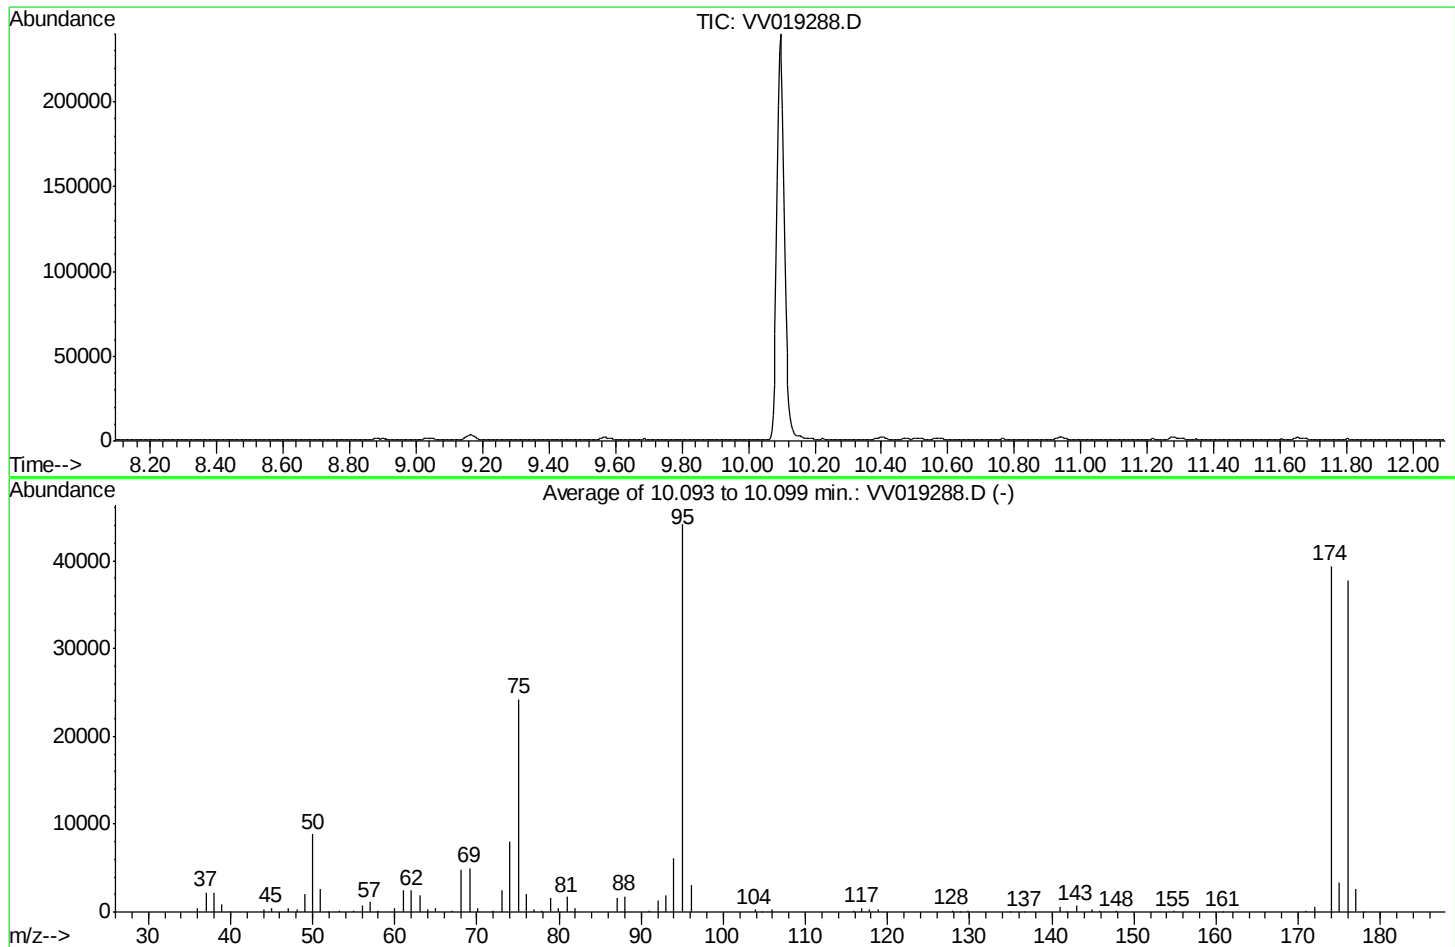

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	8880	PASS
75	95	30	80	54.9	24237	PASS
95	95	100	100	100.0	44136	PASS
96	95	5	9	6.9	3058	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.3	39410	PASS
175	174	5	9	8.5	3355	PASS
176	174	95	101	95.7	37701	PASS
177	176	5	9	6.9	2609	PASS

m/z	Abundance
36.00	423.0
37.00	2263.0
38.00	2235.0
39.00	927.0
39.90	158.0
44.00	1000.0
45.00	497.0
47.10	508.0
48.10	269.0
49.00	2065.0
50.00	8834.0
51.00	2711.0
53.20	135.0
55.00	154.0
56.10	824.0
57.00	1170.0
58.10	102.0
60.00	471.0
61.00	2487.0
62.00	2477.0
63.10	1790.0
64.00	340.0
65.00	411.0
67.10	188.0
68.00	4777.0
69.10	4981.0
70.00	370.0
71.90	253.0
73.00	2372.0
74.00	7859.0
75.10	24160.0
76.00	1960.0
77.00	296.0
78.00	213.0
78.90	1686.0
79.90	498.0
81.00	1676.0
81.90	497.0
87.00	1755.0
88.00	1801.0
90.90	205.0
92.00	1368.0
93.00	1916.0
94.00	6020.0
95.10	43648.0
96.10	2994.0
103.90	279.0
104.70	110.0
105.90	195.0
115.90	214.0
116.90	433.0
117.90	248.0
118.90	251.0
127.90	179.0
128.80	104.0
129.80	172.0
140.90	566.0
141.80	102.0
143.00	710.0
144.90	280.0
145.90	111.0
147.90	145.0
154.90	111.0
170.90	160.0
172.00	551.0
174.00	38944.0
175.00	3219.0
176.00	36776.0
177.00	2471.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.00	397.0
37.10	2254.0
38.10	2254.0
39.00	936.0
39.90	173.0
44.00	1092.0
45.00	506.0
47.10	443.0
48.10	294.0
49.10	2032.0
50.00	9150.0
51.00	2758.0
53.20	114.0
55.00	135.0
56.10	851.0
57.00	1129.0
58.00	133.0
60.00	450.0
61.00	2523.0
62.00	2543.0
63.10	1970.0
64.00	339.0
65.00	416.0
67.00	123.0
68.00	4930.0
69.10	5161.0
70.10	391.0
72.00	215.0
73.00	2503.0
74.00	8320.0
75.10	25048.0
76.00	2151.0
77.00	316.0
78.00	202.0
78.90	1696.0
80.00	491.0
80.90	1750.0
81.90	502.0
87.00	1673.0
88.00	1837.0
90.90	211.0
92.00	1396.0
93.00	1990.0
94.00	6406.0
95.00	45592.0
96.10	3180.0
103.90	283.0
104.70	110.0
105.90	243.0
115.90	229.0
116.80	465.0
117.80	250.0
118.90	297.0
127.90	193.0
129.80	193.0
134.90	101.0
136.70	112.0
141.00	575.0
143.00	726.0
144.90	262.0
145.90	126.0
147.90	146.0
154.80	123.0
171.00	133.0
172.00	608.0
174.00	40768.0
175.00	3498.0
176.00	38968.0
177.00	2749.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.00	370.0
37.10	2057.0
38.00	1970.0
39.00	879.0
39.90	175.0
44.00	1122.0
45.00	482.0
47.10	385.0
48.00	319.0
49.10	1909.0
50.00	8657.0
51.00	2492.0
51.90	109.0
55.10	127.0
56.00	742.0
57.00	1058.0
57.90	113.0
59.90	427.0
61.00	2366.0
62.00	2408.0
63.00	1964.0
64.00	309.0
65.00	448.0
67.00	103.0
68.00	4614.0
69.10	4738.0
70.10	373.0
72.00	197.0
73.00	2416.0
74.00	8011.0
75.10	23504.0
76.00	2090.0
77.00	286.0
77.90	191.0
78.90	1504.0
80.00	466.0
80.90	1666.0
81.90	427.0
87.00	1558.0
88.00	1636.0
90.90	193.0
92.00	1283.0
93.00	1986.0
94.00	6023.0
95.00	43168.0
96.10	3001.0
103.90	226.0
105.90	239.0
115.90	213.0
116.80	432.0
117.80	212.0
118.90	310.0
127.90	196.0
129.80	175.0
134.90	112.0
136.70	117.0
140.90	515.0
142.90	687.0
144.90	217.0
145.80	119.0
147.90	129.0
154.80	126.0
160.80	106.0
171.90	607.0
174.00	38520.0
175.00	3349.0
176.00	37360.0
177.00	2609.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

Scan 2789 (10.058 min): VV019288.D
BFB90

m/z	Abundance
40.00	137.0
44.00	739.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90