

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110821\
 Data File : VW023279.D
 Acq On : 08 Nov 2021 15:23
 Operator : SY/MD
 Sample : M4445-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3A3

Quant Time: Nov 09 05:16:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 05:13:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	128834	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	133119	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62020	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	35399	4.386	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.800%
7) Chloroethane-d5	1.568	69	32504	4.941	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%
11) 1,1-Dichloroethene-d2	2.111	63	51417	3.403	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.889	46	86472	62.189	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.380%
24) Chloroform-d	4.352	84	82245	4.782	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.034	65	40012	5.173	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%
32) Benzene-d6	5.053	84	155964	4.566	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	6.072	67	48681	4.842	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.800%
41) Toluene-d8	7.317	98	133163	4.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.200%
43) trans-1,3-Dichloroprop...	7.625	79	17123	4.491	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.800%
46) 2-Hexanone-d5	8.088	63	63360	45.169	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.340%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33952	4.696	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	52267	5.061	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds					Qvalue	
13) Acetone	2.182	43	3170	3.731	ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023279.D
Acq On : 08 Nov 2021 15:23
Operator : SY/MD
Sample : M4445-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A3

Quant Time: Nov 09 05:16:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 05:13:22 2021
Response via : Initial Calibration

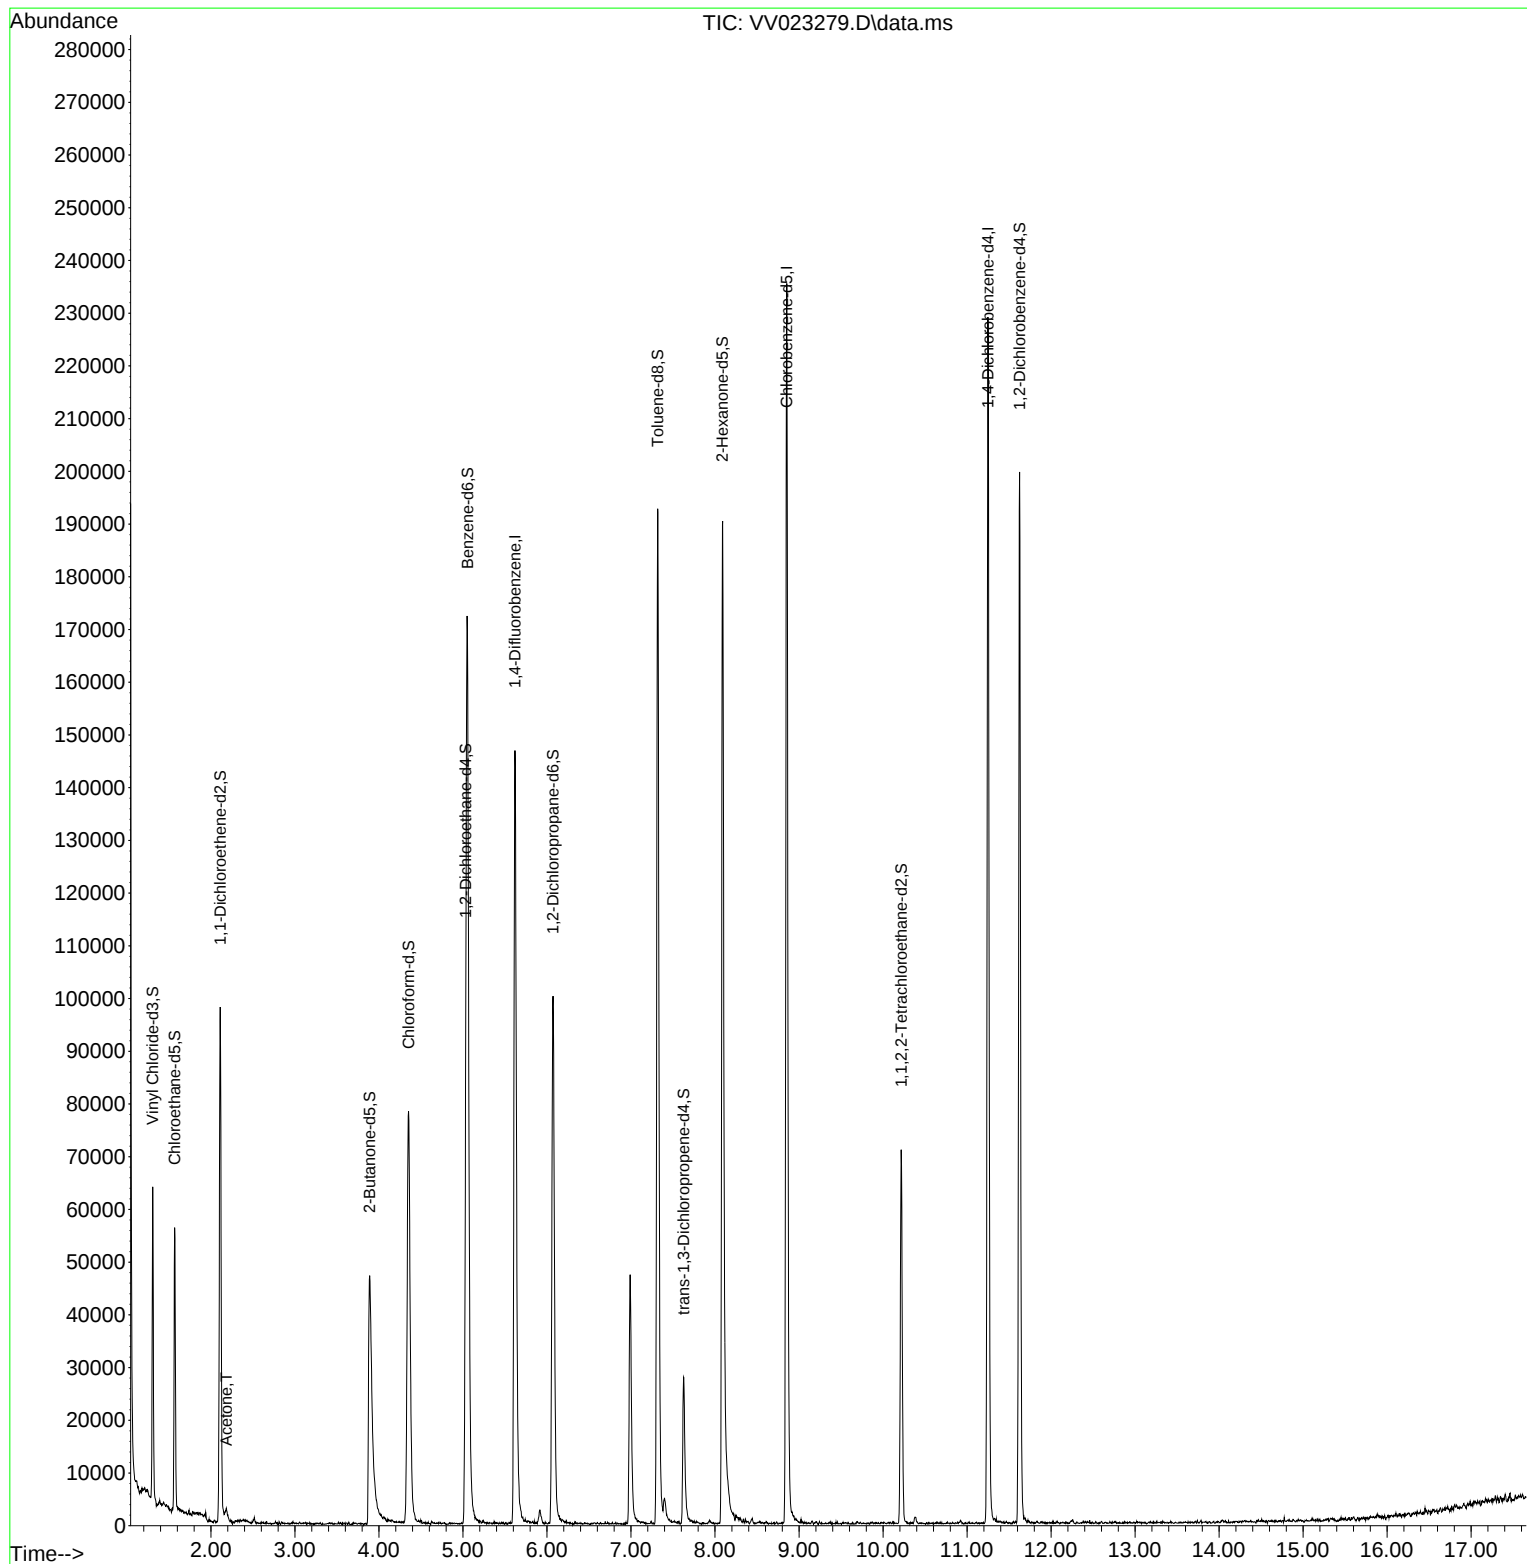

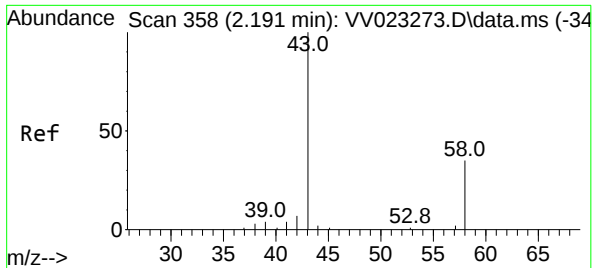

#13
 Acetone
 Concen: 3.731 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV023279.D
 Acq: 08 Nov 2021 15:23

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3A3

Tgt Ion: 43 Resp: 3170
 Ion Ratio Lower Upper
 43 100
 58 15.0 0.0 55.4

