

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110821\
 Data File : VW023285.D
 Acq On : 08 Nov 2021 17:44
 Operator : SY/MD
 Sample : M4522-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG330

Quant Time: Nov 09 05:17:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 05:13:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129291	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	131176	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60157	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	31893	3.938	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.800%	
7) Chloroethane-d5	1.568	69	29349	4.446	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.000%	
11) 1,1-Dichloroethene-d2	2.108	63	47842	3.155	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.886	46	83086	59.542	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	119.080%	
24) Chloroform-d	4.352	84	78446	4.545	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
26) 1,2-Dichloroethane-d4	5.034	65	38019	4.898	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.000%	
32) Benzene-d6	5.053	84	146670	4.358	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.200%	
36) 1,2-Dichloropropane-d6	6.072	67	47257	4.770	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.400%	
41) Toluene-d8	7.320	98	123999	3.932	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	7.625	79	16435	4.375	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.088	63	62684	45.349	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.700%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31929	4.481	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	89.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	48817	4.873	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.400%	
Target Compounds					Qvalue	
13) Acetone	2.179	43	1852	2.172	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023285.D
Acq On : 08 Nov 2021 17:44
Operator : SY/MD
Sample : M4522-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG330


Quant Time: Nov 09 05:17:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 05:13:22 2021
Response via : Initial Calibration

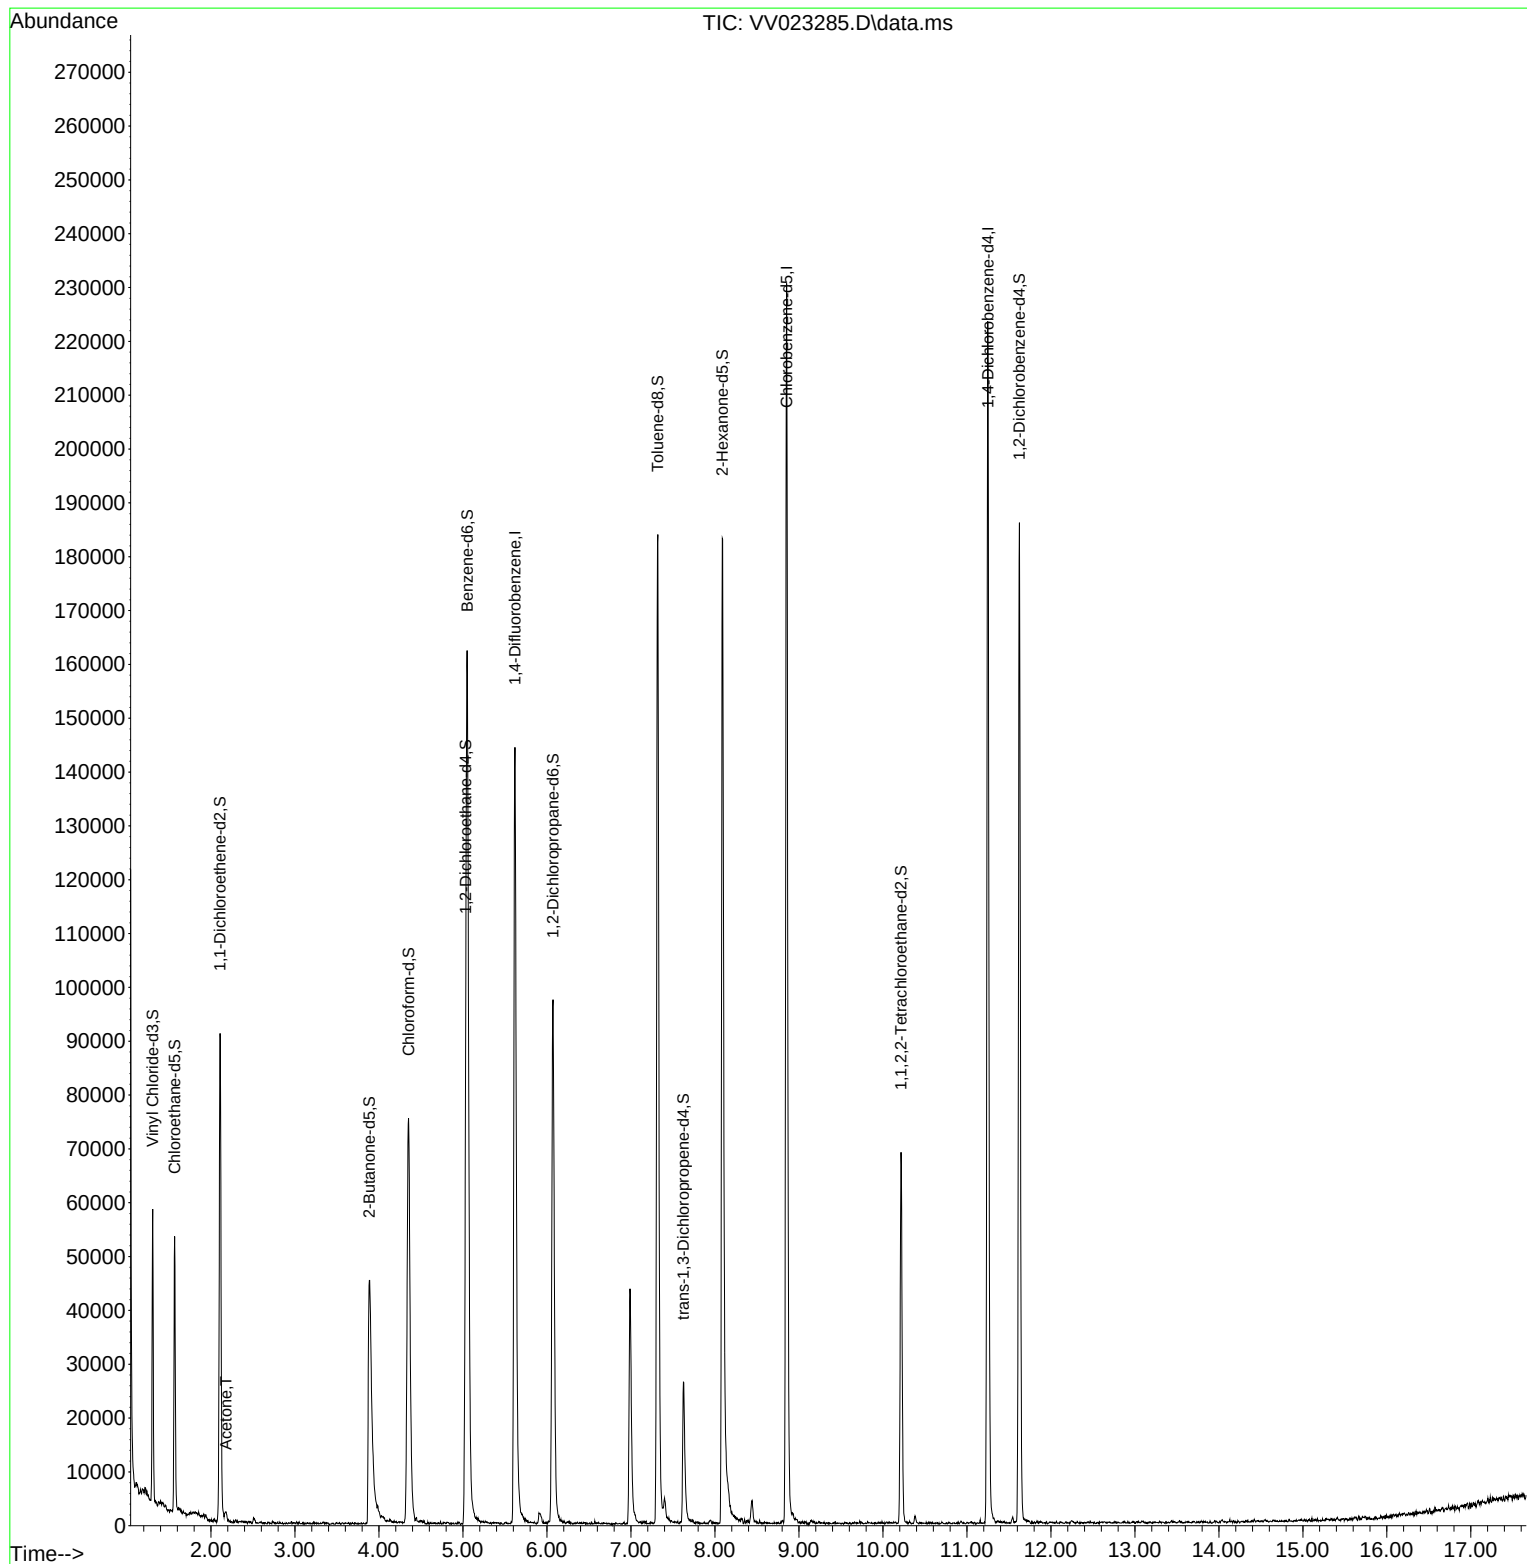

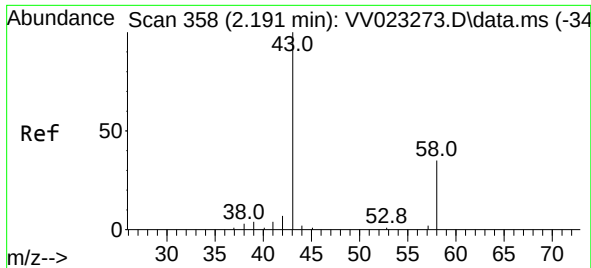

#13
 Acetone
 Concen: 2.172 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV023285.D
 Acq: 08 Nov 2021 17:44

Instrument :
 MSVOA_V
 ClientSampleId :
 BG330

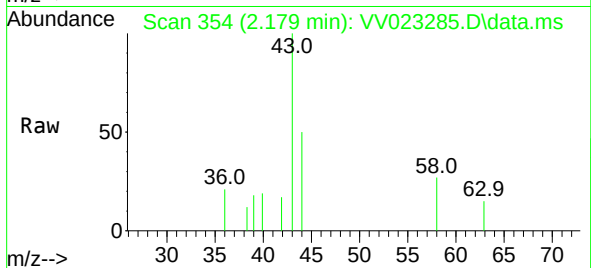

Tgt Ion: 43 Resp: 1852
 Ion Ratio Lower Upper
 43 100
 58 26.8 0.0 55.4

