

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110821\
 Data File : VW023288.D
 Acq On : 08 Nov 2021 18:54
 Operator : SY/MD
 Sample : M4522-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG393

Quant Time: Nov 09 05:18:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 05:13:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123905	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125147	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58330	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	30766	3.964	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.568	69	27988	4.424	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.400%
11) 1,1-Dichloroethene-d2	2.108	63	44398	3.055	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.200%
20) 2-Butanone-d5	3.883	46	79106	59.154	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.300%
24) Chloroform-d	4.352	84	74485	4.503	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.034	65	37115	4.989	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	5.053	84	143042	4.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.072	67	45426	4.806	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.320	98	117465	3.904	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	7.625	79	15039	4.196	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.088	63	57993	43.977	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31749	4.671	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	46151	4.752	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds						
					Qvalue	
13) Acetone	2.172	43	4245	5.195	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023288.D
Acq On : 08 Nov 2021 18:54
Operator : SY/MD
Sample : M4522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG393

Quant Time: Nov 09 05:18:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 05:13:22 2021
Response via : Initial Calibration

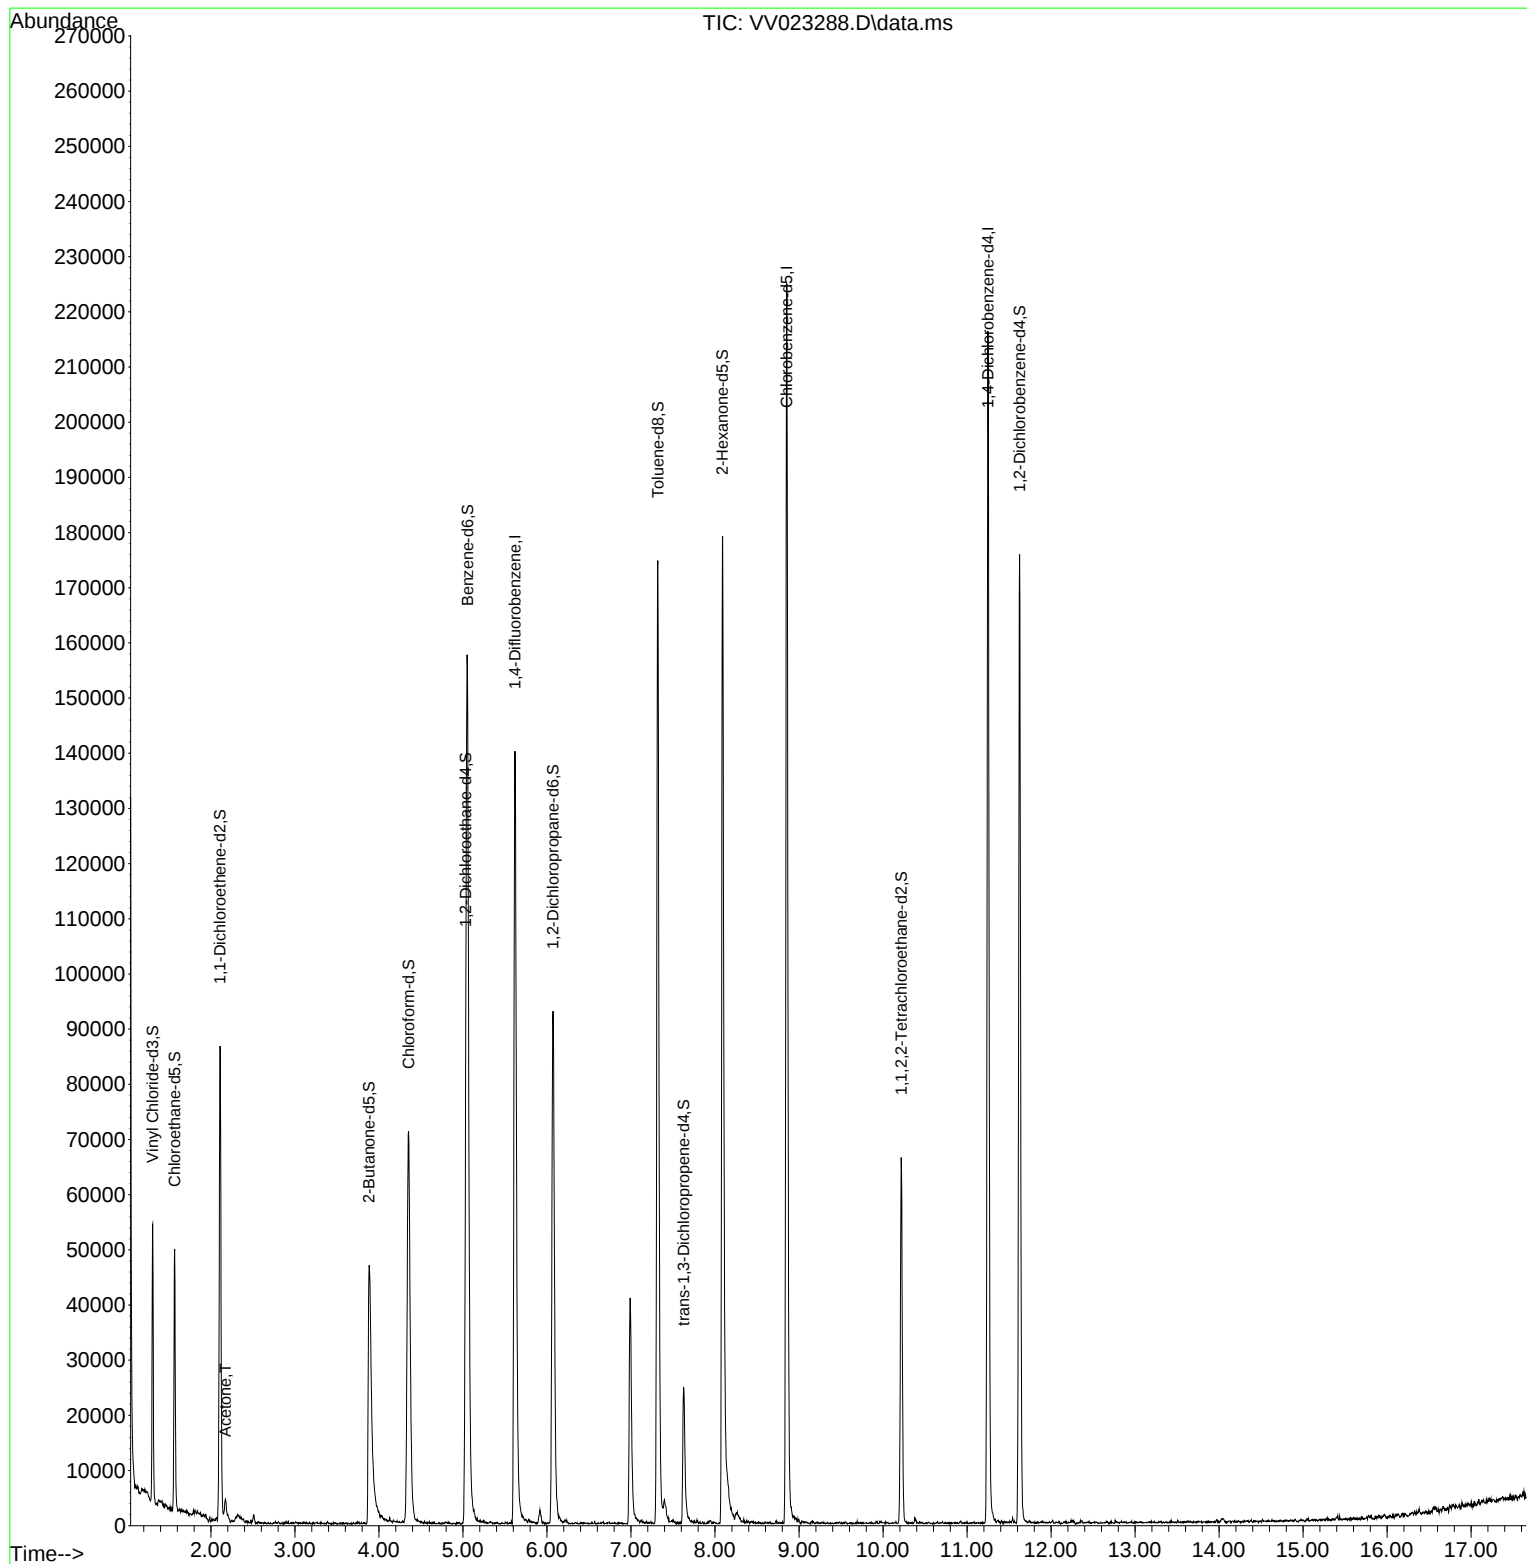

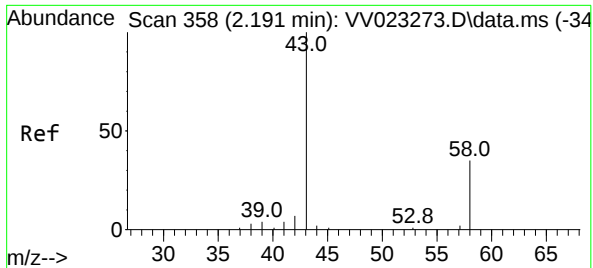

#13
 Acetone
 Concen: 5.195 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV023288.D
 Acq: 08 Nov 2021 18:54

Instrument :
 MSVOA_V
 ClientSampleId :
 BG393

Tgt Ion: 43 Resp: 4245
 Ion Ratio Lower Upper
 43 100
 58 28.5 0.0 55.4

