

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110821\
 Data File : VW023289.D
 Acq On : 08 Nov 2021 19:18
 Operator : SY/MD
 Sample : M4522-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG394

Quant Time: Nov 09 05:18:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 05:13:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117011	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	118318	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54644	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	31245	4.262	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.200%	
7) Chloroethane-d5	1.568	69	27706	4.638	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.800%	
11) 1,1-Dichloroethene-d2	2.108	63	44462	3.240	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.800%	
20) 2-Butanone-d5	3.883	46	80791	63.974	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	127.940%	
24) Chloroform-d	4.352	84	75037	4.803	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.000%	
26) 1,2-Dichloroethane-d4	5.034	65	35999	5.124	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.400%	
32) Benzene-d6	5.053	84	141128	4.649	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.072	67	44718	5.004	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.317	98	116445	4.093	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.800%	
43) trans-1,3-Dichloroprop...	7.628	79	14692	4.336	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.800%	
46) 2-Hexanone-d5	8.088	63	57403	46.042	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.080%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30867	4.803	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	46587	5.120	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.400%	
Target Compounds					Qvalue	
13) Acetone	2.172	43	2272	2.944	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023289.D
Acq On : 08 Nov 2021 19:18
Operator : SY/MD
Sample : M4522-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG394

Quant Time: Nov 09 05:18:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 05:13:22 2021
Response via : Initial Calibration

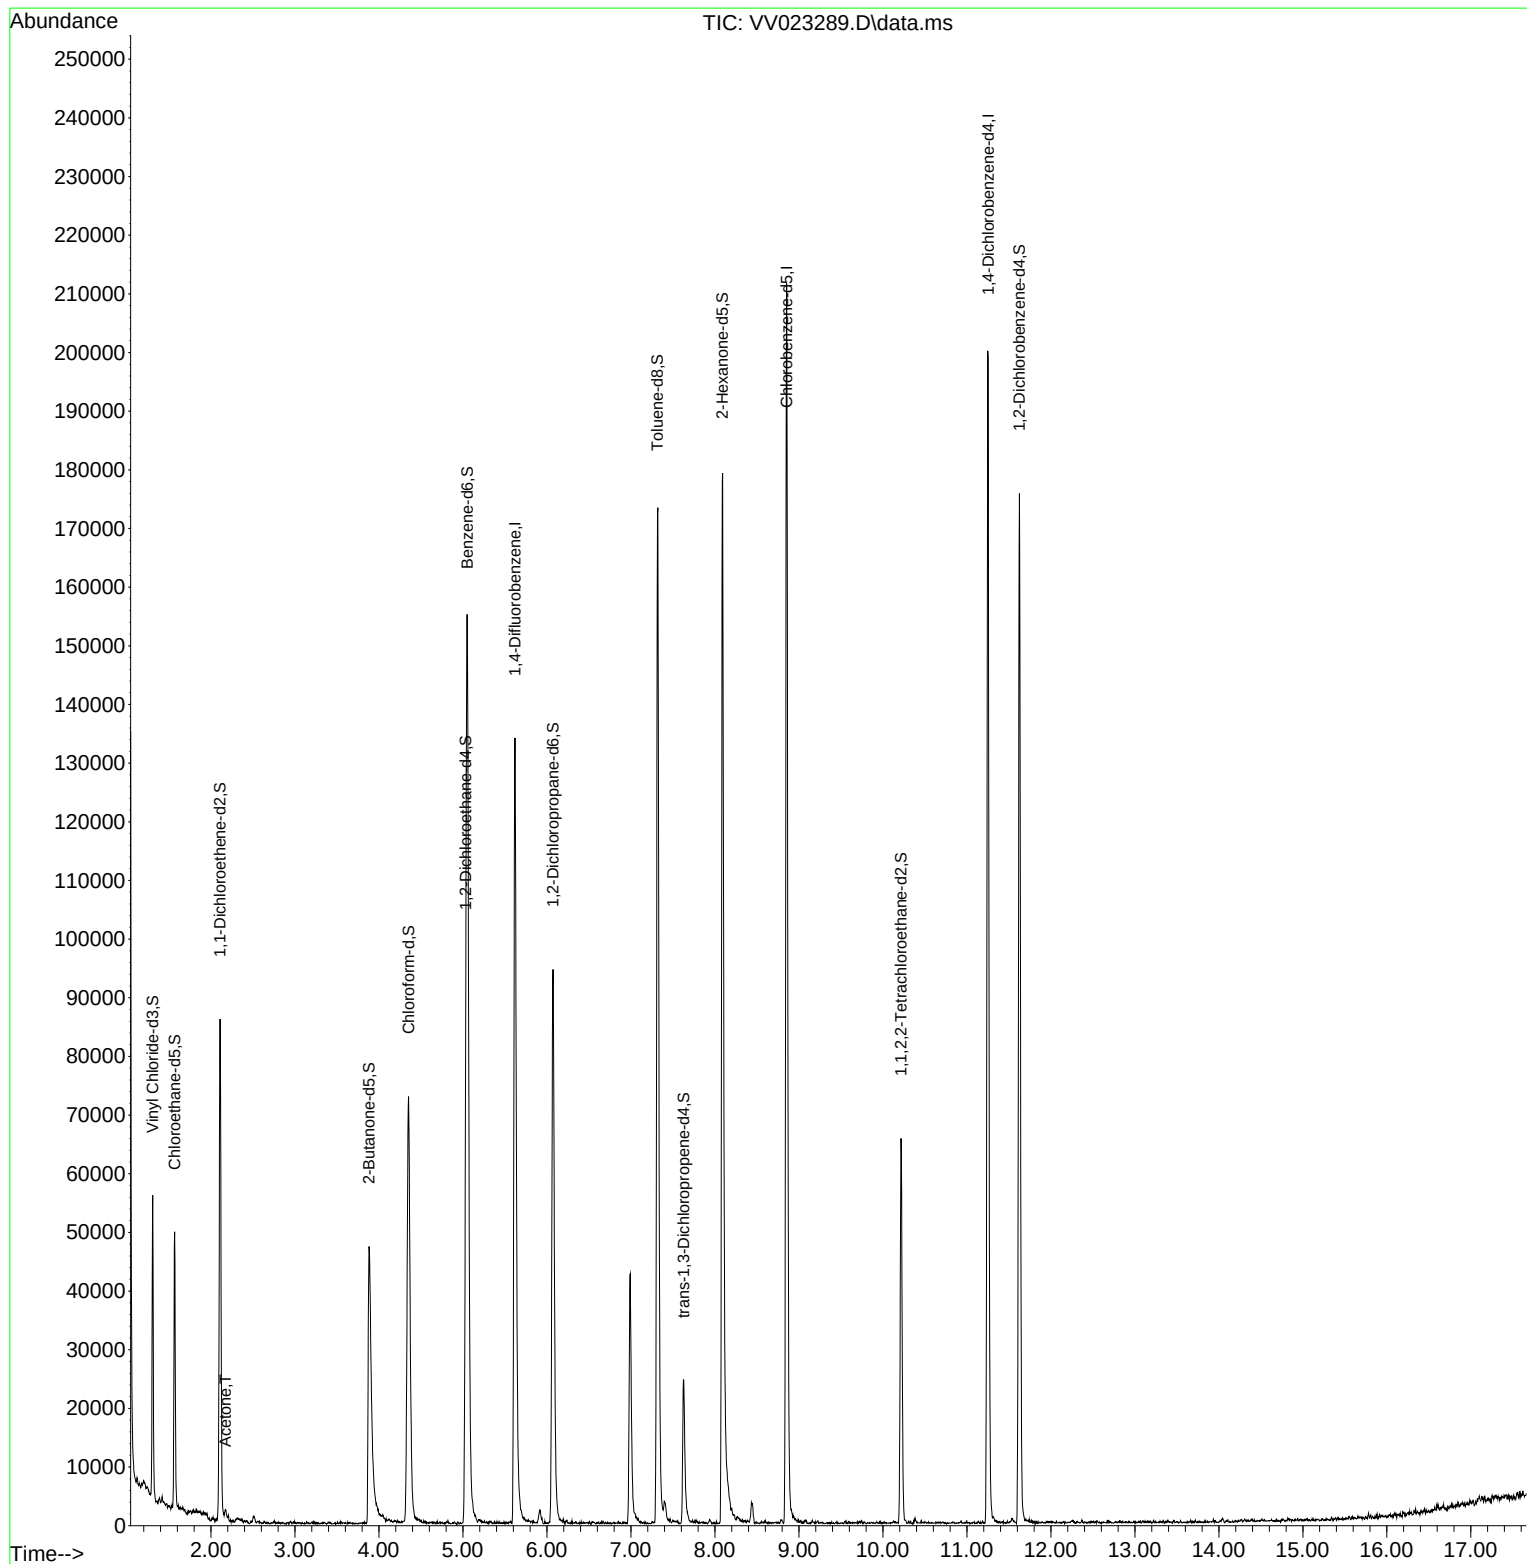

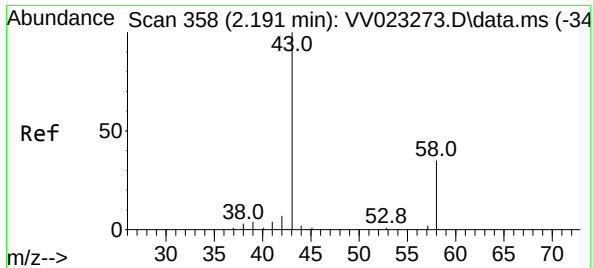

#13
 Acetone
 Concen: 2.944 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV023289.D
 Acq: 08 Nov 2021 19:18

Instrument :
 MSVOA_V
 ClientSampleId :
 BG394

Tgt Ion: 43 Resp: 2272
 Ion Ratio Lower Upper
 43 100
 58 30.2 0.0 55.4

