

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110821\
 Data File : VW023290.D
 Acq On : 08 Nov 2021 19:41
 Operator : SY/MD
 Sample : M4522-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG395

Quant Time: Nov 09 05:18:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 05:13:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122166	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	125138	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58101	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	30787	4.023	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.400%
7) Chloroethane-d5	1.568	69	28336	4.543	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.800%
11) 1,1-Dichloroethene-d2	2.108	63	44331	3.094	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.800%
20) 2-Butanone-d5	3.886	46	84659	64.208	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.420%
24) Chloroform-d	4.352	84	75381	4.622	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
26) 1,2-Dichloroethane-d4	5.034	65	36380	4.960	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.053	84	140358	4.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
36) 1,2-Dichloropropane-d6	6.069	67	45507	4.815	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.317	98	117473	3.904	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	7.629	79	15733	4.390	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.800%
46) 2-Hexanone-d5	8.088	63	59252	44.935	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.860%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29996	4.413	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	46785	4.836	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
13) Acetone	2.175	43	1947	2.417	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023290.D
Acq On : 08 Nov 2021 19:41
Operator : SY/MD
Sample : M4522-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG395

Quant Time: Nov 09 05:18:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 05:13:22 2021
Response via : Initial Calibration

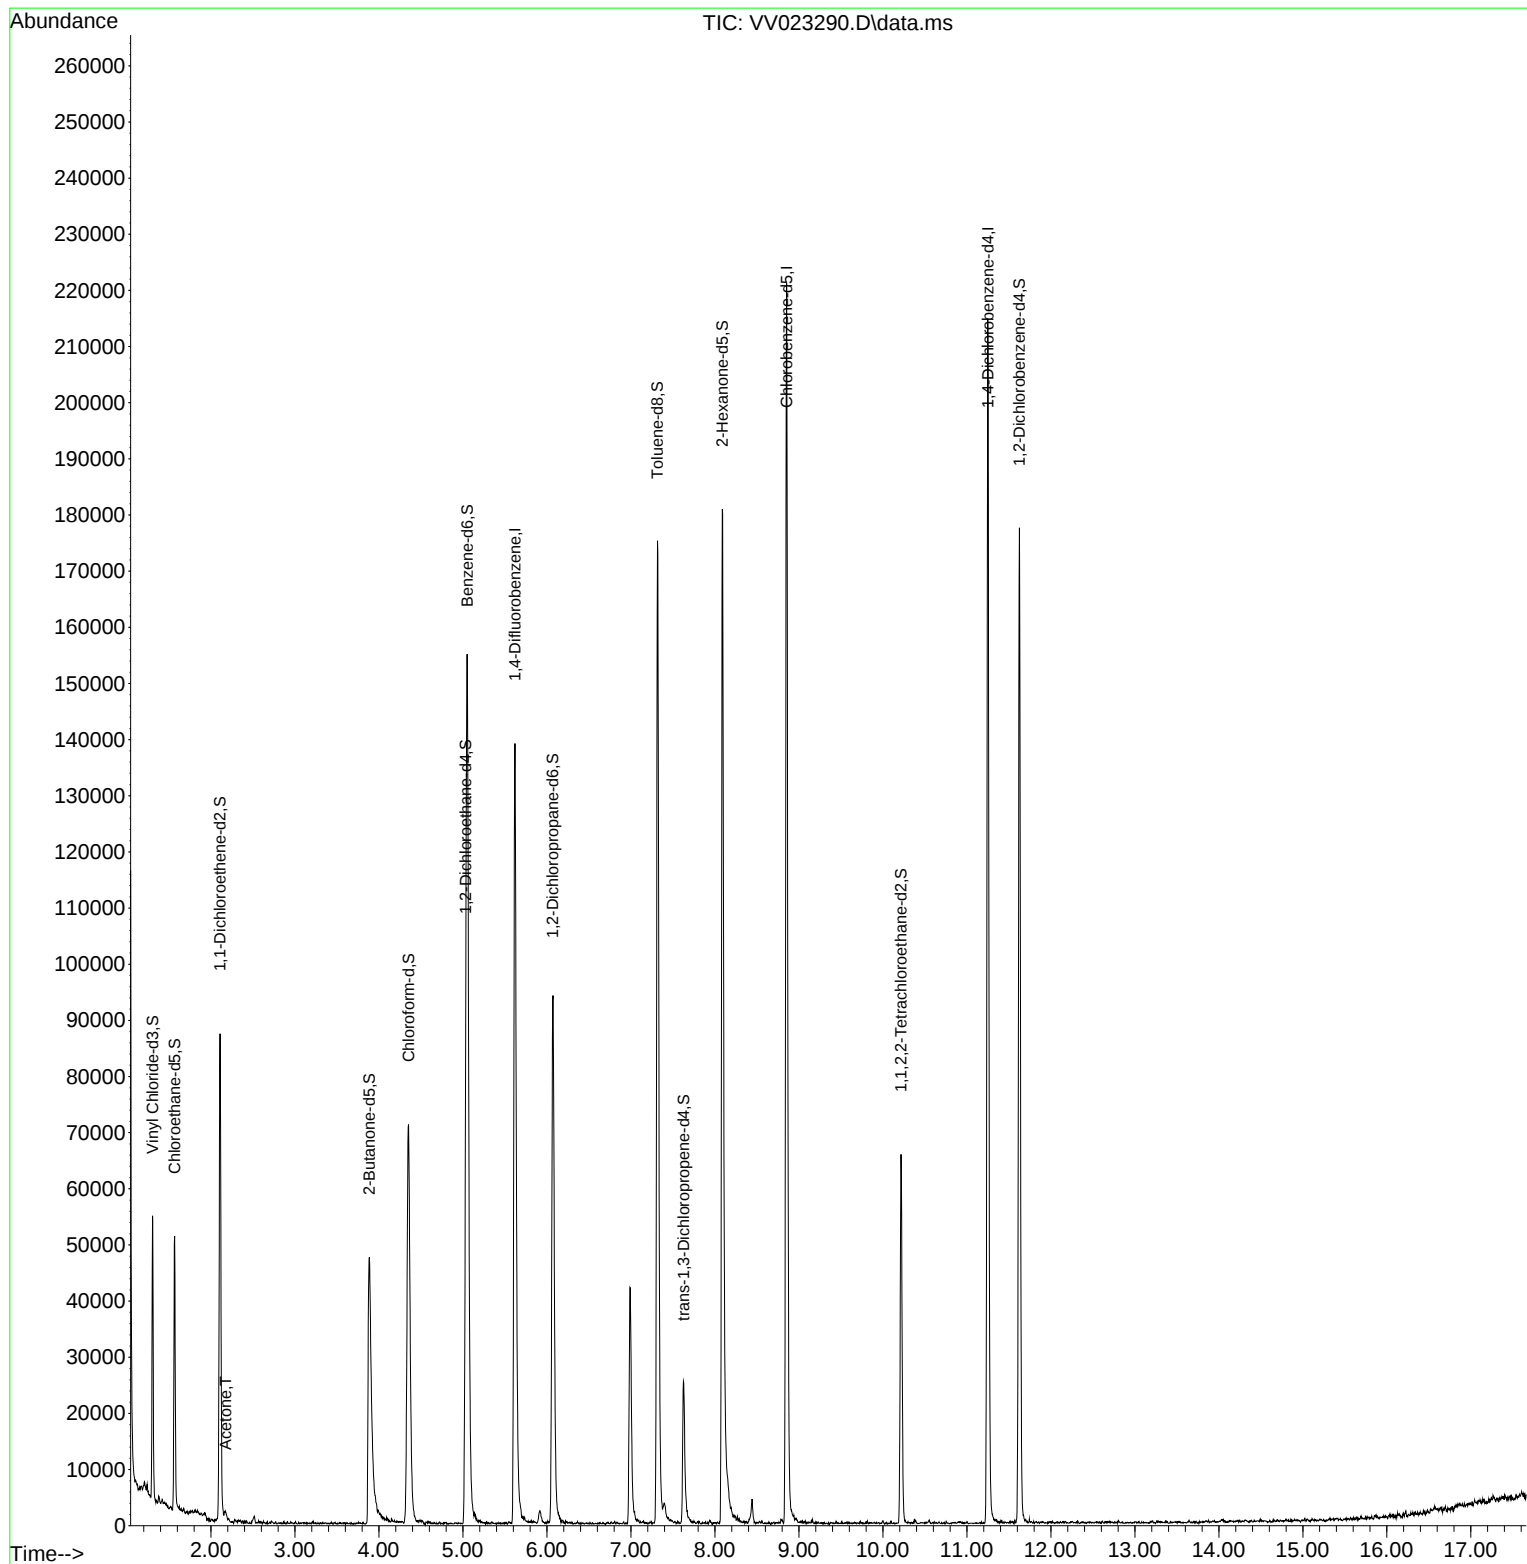

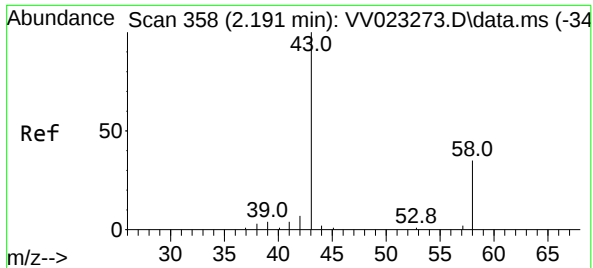

#13
 Acetone
 Concen: 2.417 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV023290.D
 Acq: 08 Nov 2021 19:41

Instrument :
 MSVOA_V
 ClientSampleId :
 BG395

Tgt Ion: 43 Resp: 1947
 Ion Ratio Lower Upper
 43 100
 58 28.5 0.0 55.4

