

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
 Data File : VV023276.D
 Acq On : 08 Nov 2021 14:07
 Operator : SY/MD
 Sample : M4492-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1S2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	72	rVB	4075	5349	1.17%	0.140%
2	1.304	76	82	93	rVB	62319	61167	13.43%	1.599%
3	1.564	156	163	175	rBV	54430	62956	13.82%	1.645%
4	2.105	320	331	344	rBV	103949	152060	33.38%	3.974%
5	3.899	877	889	926	rBV2	35303	135205	29.68%	3.533%
6	4.346	1010	1028	1060	rBV3	89990	265093	58.20%	6.928%
7	5.043	1229	1245	1273	rBV2	178210	455500	100.00%	11.904%
8	5.612	1410	1422	1450	rBV	154744	318528	69.93%	8.325%
9	5.911	1504	1515	1537	rBV2	45894	97253	21.35%	2.542%
10	6.066	1549	1563	1590	rBV	101881	215378	47.28%	5.629%
11	6.985	1839	1849	1867	rBV	47051	88517	19.43%	2.313%
12	7.313	1938	1951	1969	rBV	199112	353612	77.63%	9.241%
13	7.622	2036	2047	2067	rBV	28524	52746	11.58%	1.378%
14	8.088	2182	2192	2231	rBV	171199	362950	79.68%	9.485%
15	8.850	2418	2429	2452	rBV	235076	393264	86.34%	10.278%
16	10.217	2843	2854	2869	rBV	71265	113370	24.89%	2.963%
17	10.381	2893	2905	2914	rVB3	4081	6216	1.36%	0.162%
18	11.249	3164	3175	3195	rBV	227456	355683	78.09%	9.296%
19	11.532	3253	3263	3281	rBV4	8452	15107	3.32%	0.395%
20	11.625	3281	3292	3310	rVV	198081	316437	69.47%	8.270%




Sum of corrected areas: 3826391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023276.D
Acq On : 08 Nov 2021 14:07
Operator : SY/MD
Sample : M4492-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

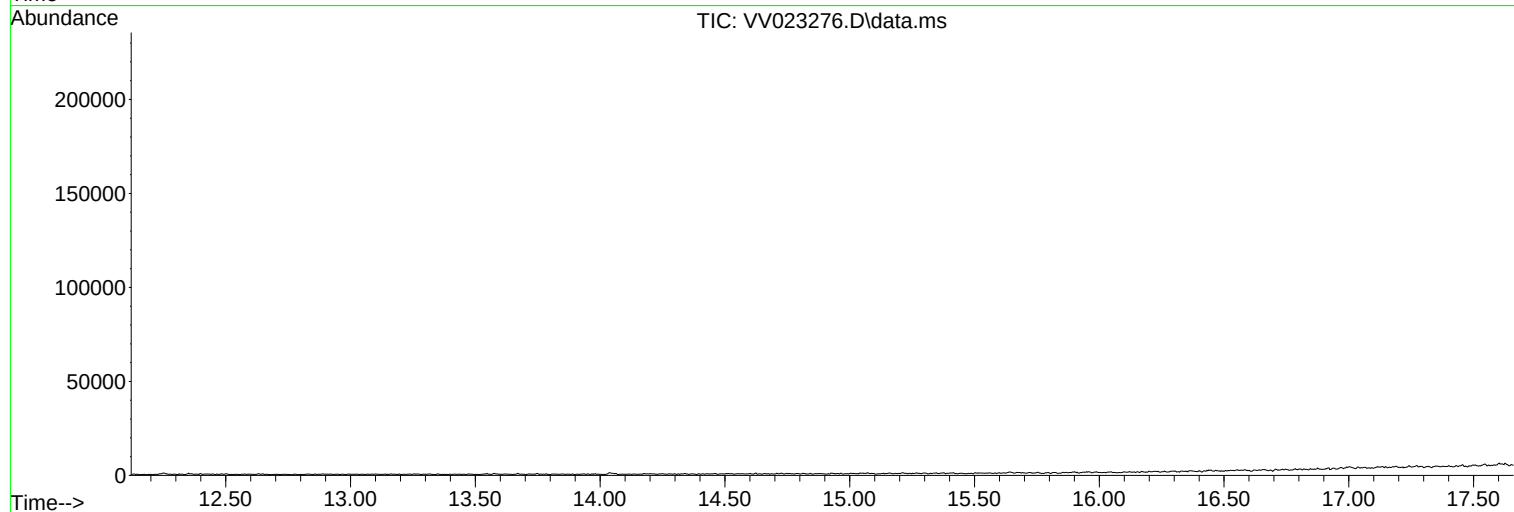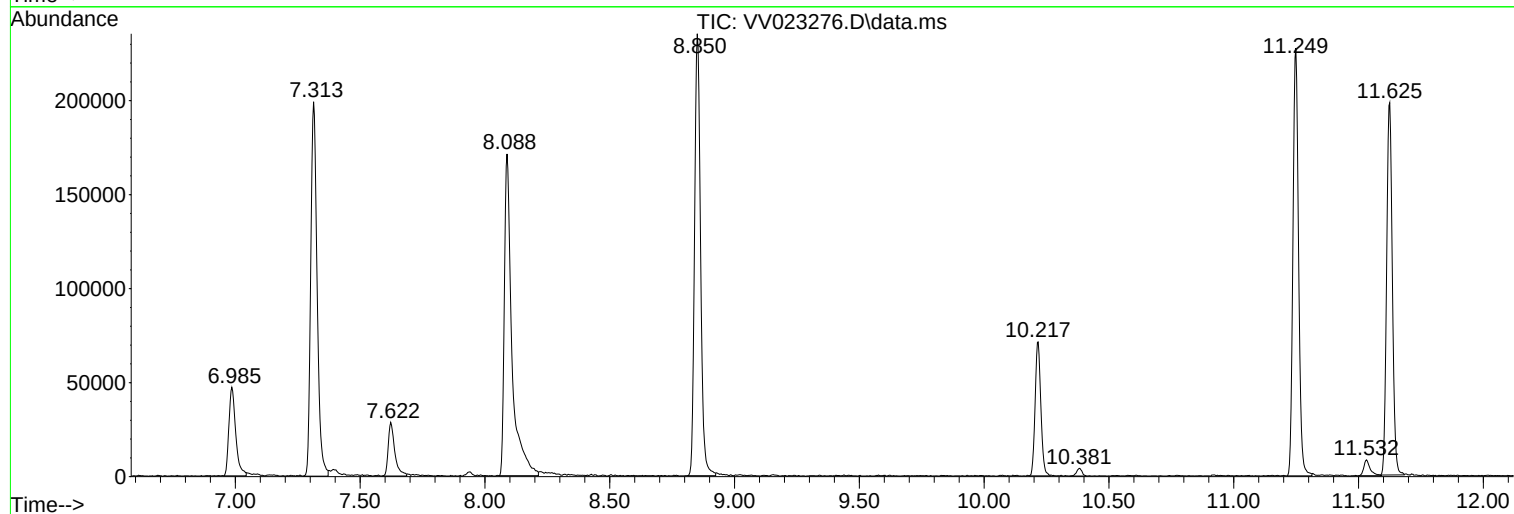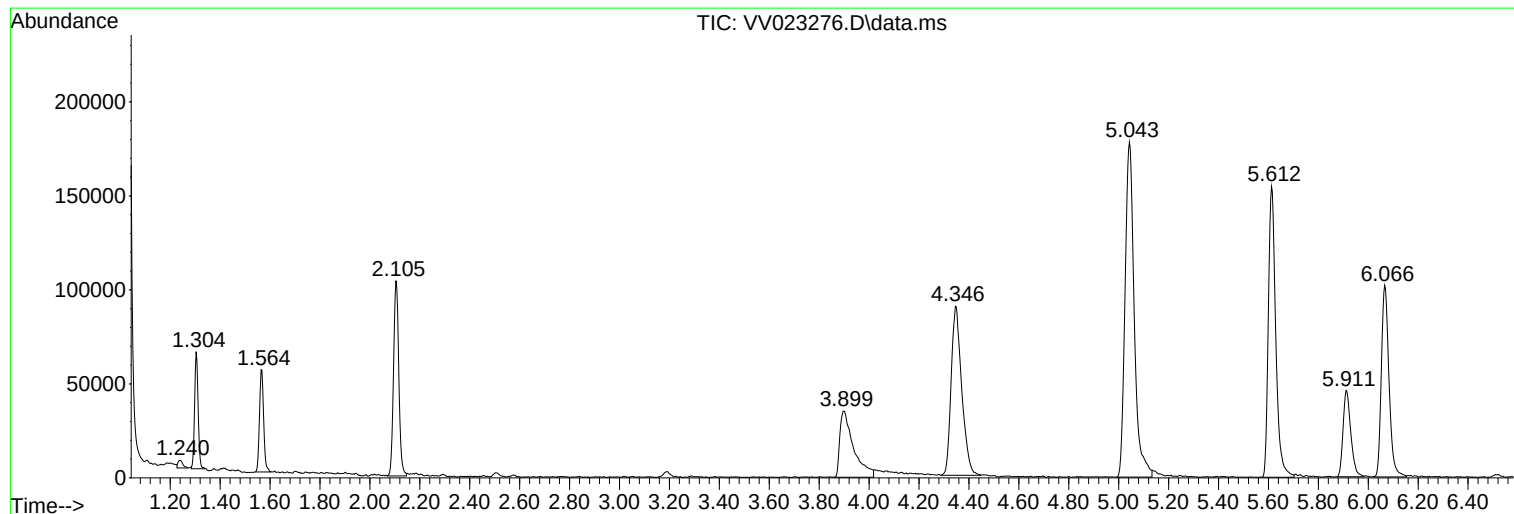

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023276.D
Acq On : 08 Nov 2021 14:07
Operator : SY/MD
Sample : M4492-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023276.D
Acq On : 08 Nov 2021 14:07
Operator : SY/MD
Sample : M4492-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc