

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
 Data File : VV023277.D
 Acq On : 08 Nov 2021 14:30
 Operator : SY/MD
 Sample : M4492-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1R8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	60515	64035	14.00%	1.671%
2	1.568	157	164	175	rVB	54019	60523	13.23%	1.579%
3	2.018	292	304	314	rBV	24926	36566	7.99%	0.954%
4	2.108	322	332	348	rBV	102229	148362	32.43%	3.871%
5	3.908	881	892	922	rBV	34190	130459	28.52%	3.404%
6	4.349	1012	1029	1057	rVB2	81922	200342	43.80%	5.227%
7	5.050	1230	1247	1281	rBV3	174821	457451	100.00%	11.935%
8	5.619	1412	1424	1448	rBV	143020	290202	63.44%	7.571%
9	5.918	1504	1517	1550	rBV2	93958	193408	42.28%	5.046%
10	6.072	1551	1565	1584	rBV	102583	210702	46.06%	5.497%
11	6.989	1839	1850	1868	rBV2	45701	88761	19.40%	2.316%
12	7.317	1941	1952	1970	rBV	201822	354246	77.44%	9.242%
13	7.397	1974	1977	1993	rVB5	3486	5877	1.28%	0.153%
14	7.629	2039	2049	2065	rBV2	28740	52209	11.41%	1.362%
15	8.092	2180	2193	2233	rBV	176553	378366	82.71%	9.872%
16	8.854	2418	2430	2450	rBV	223255	366834	80.19%	9.571%
17	10.217	2842	2854	2867	rBV	71308	114615	25.06%	2.990%
18	10.384	2893	2906	2916	rBV4	3116	5071	1.11%	0.132%
19	11.249	3164	3175	3197	rBV	215380	339588	74.23%	8.860%
20	11.532	3255	3263	3278	rBV2	9379	16623	3.63%	0.434%
21	11.625	3278	3292	3307	rBV	205081	318648	69.66%	8.314%




Sum of corrected areas: 3832888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023277.D
Acq On : 08 Nov 2021 14:30
Operator : SY/MD
Sample : M4492-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1R8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

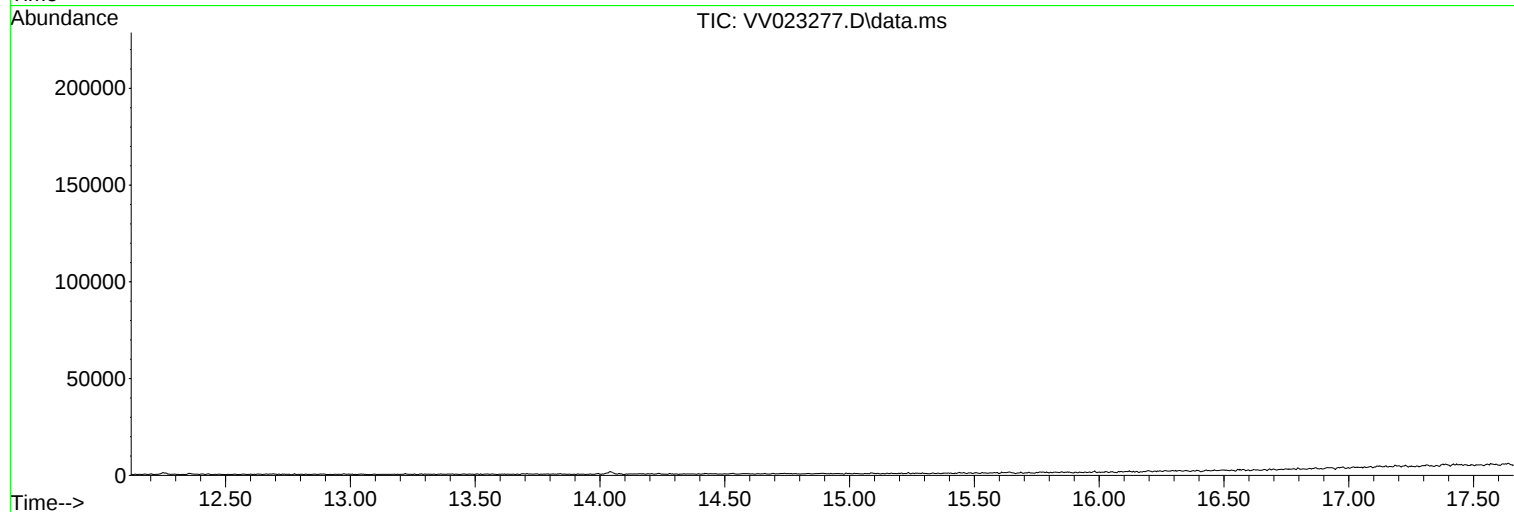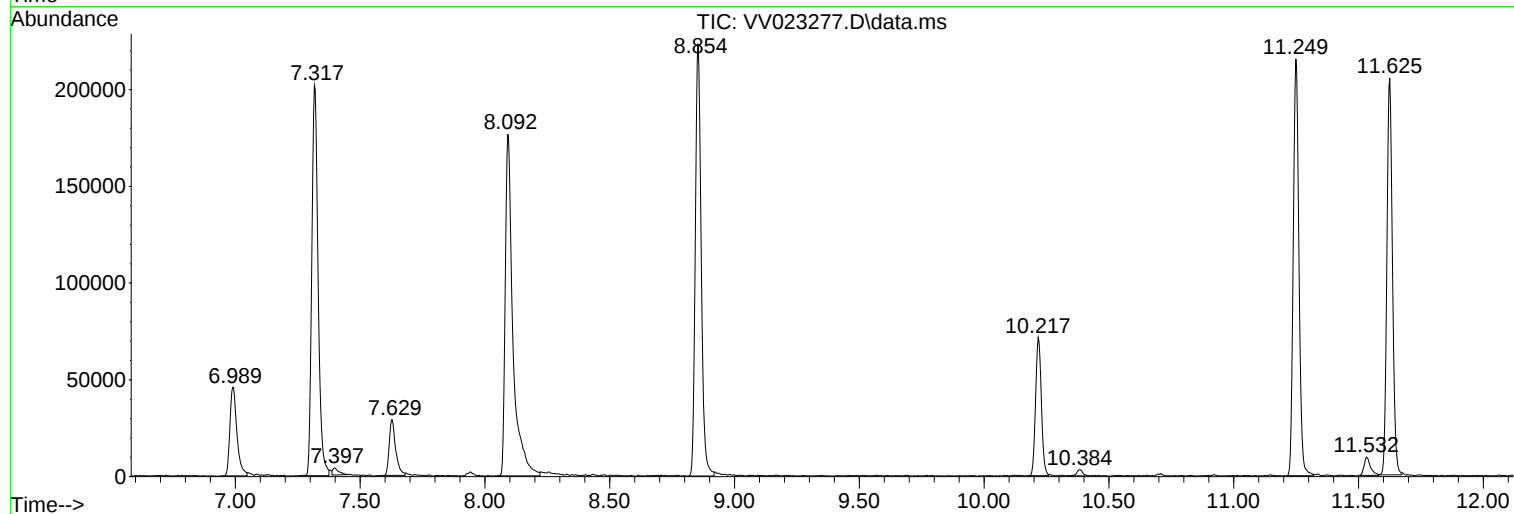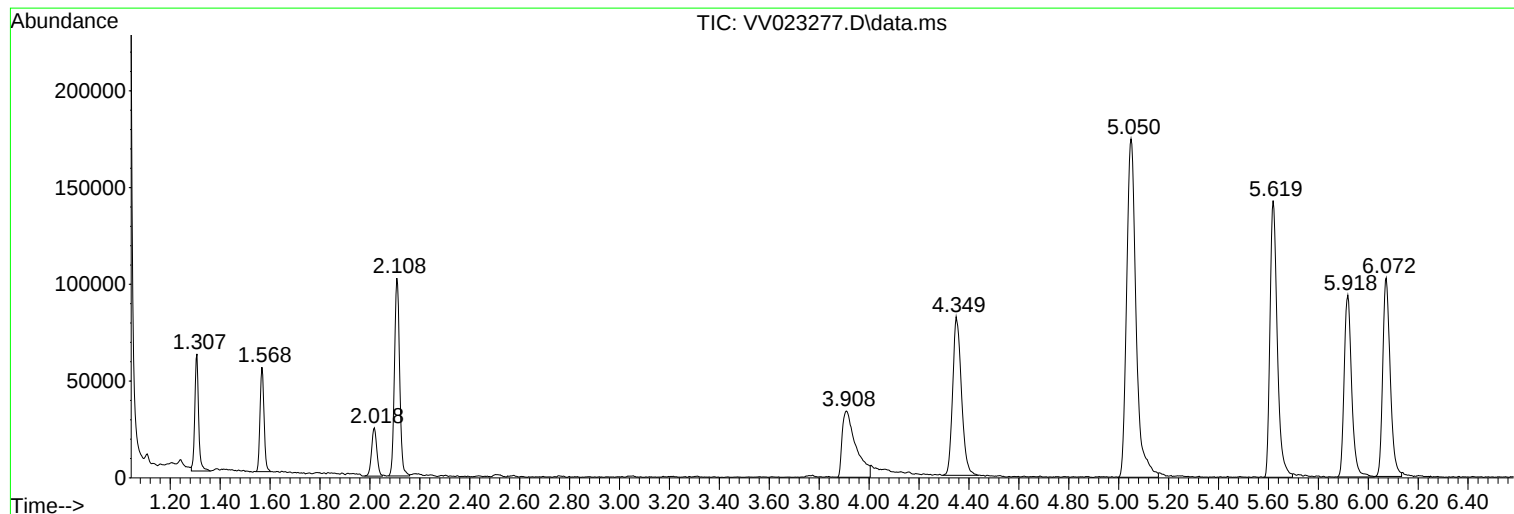

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023277.D
Acq On : 08 Nov 2021 14:30
Operator : SY/MD
Sample : M4492-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1R8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.018	0.63 ug/L	36566	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	80
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	80
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	72
4			2-Propyn-1-ol, acetate	98	C5H6O2	000627-09-8	9
5			(S)-(-)-2-Chloropropionic acid	108	C3H5ClO2	029617-66-1	9

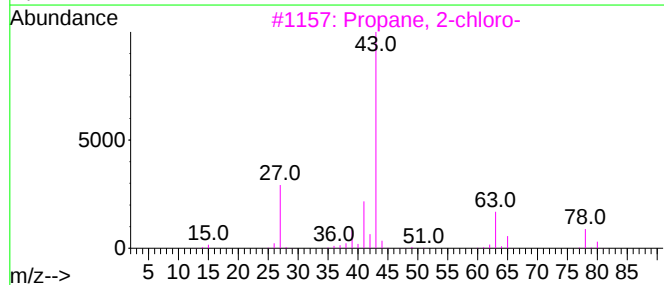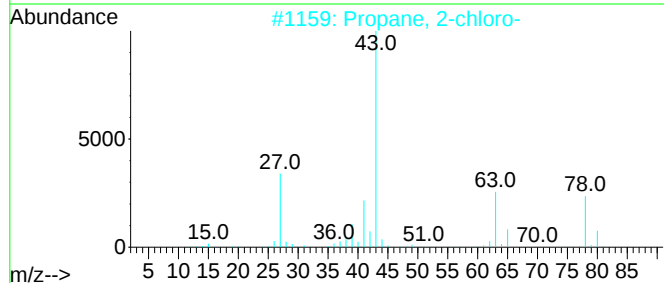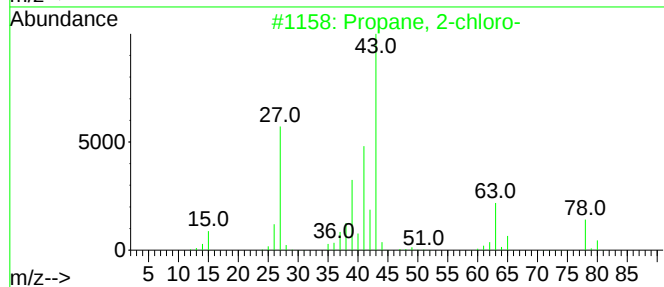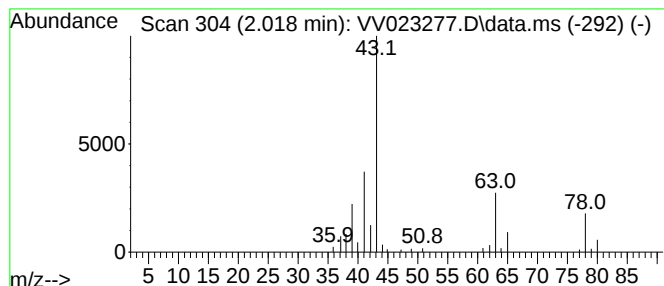

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023277.D
Acq On : 08 Nov 2021 14:30
Operator : SY/MD
Sample : M4492-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1R8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.018	0.6	ug/L	36566	1	5.619	290202	5.0