

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
 Data File : VV023281.D
 Acq On : 08 Nov 2021 16:10
 Operator : SY/MD
 Sample : M4445-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3A5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rVB	55631	56556	13.77%	1.645%
2	1.568	156	164	173	rBV	51339	57598	14.02%	1.675%
3	2.108	323	332	346	rBV	93977	134778	32.81%	3.920%
4	3.889	876	886	923	rBV	43598	136770	33.30%	3.978%
5	4.349	1012	1029	1055	rBV2	77848	189861	46.22%	5.522%
6	5.050	1230	1247	1283	rBV2	161691	410782	100.00%	11.947%
7	5.619	1412	1424	1446	rBV	144352	295167	71.85%	8.584%
8	6.072	1551	1565	1586	rBV2	96451	199263	48.51%	5.795%
9	6.989	1840	1850	1867	rBV	43570	81275	19.79%	2.364%
10	7.320	1942	1953	1970	rBV	182023	323435	78.74%	9.407%
11	7.397	1970	1977	1997	rVB	11437	23662	5.76%	0.688%
12	7.625	2038	2048	2062	rBV2	25998	47891	11.66%	1.393%
13	8.088	2182	2192	2224	rBV	178673	341992	83.25%	9.946%
14	8.442	2292	2302	2309	rBV6	3681	6098	1.48%	0.177%
15	8.854	2419	2430	2452	rBV	232220	378054	92.03%	10.995%
16	9.149	2513	2522	2534	rBV5	4840	8045	1.96%	0.234%
17	10.217	2843	2854	2867	rBV2	67706	107007	26.05%	3.112%
18	11.249	3165	3175	3193	rBV	224282	347438	84.58%	10.105%
19	11.625	3280	3292	3313	rBV	186845	292746	71.27%	8.514%




Sum of corrected areas: 3438418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023281.D
Acq On : 08 Nov 2021 16:10
Operator : SY/MD
Sample : M4445-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

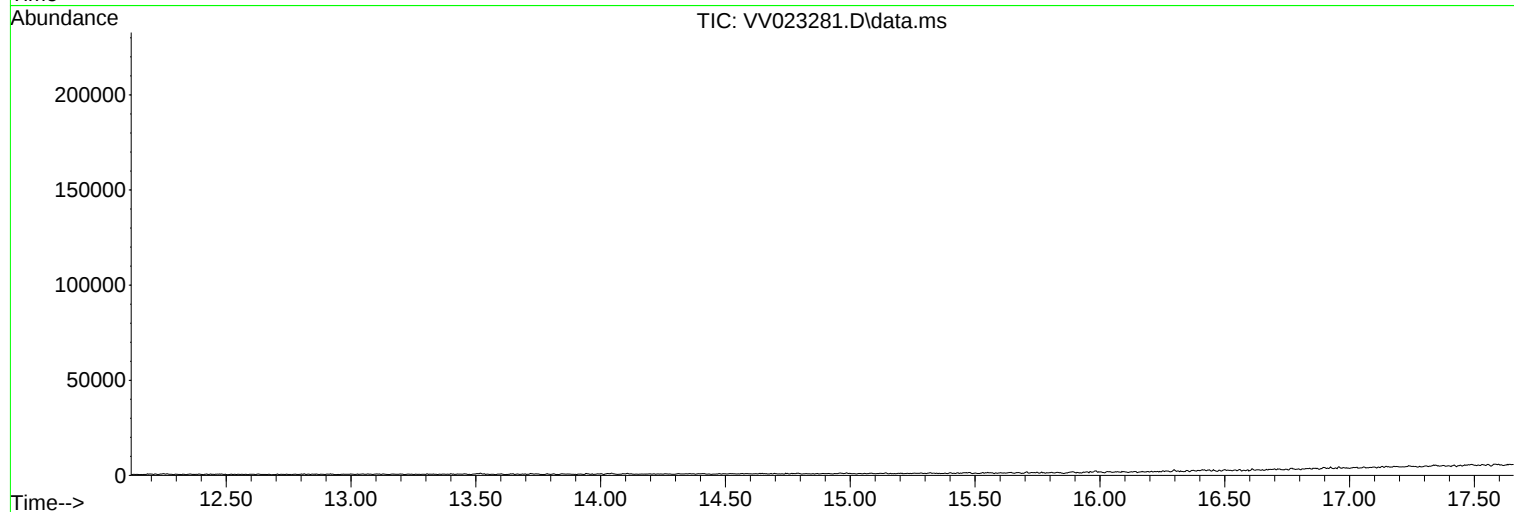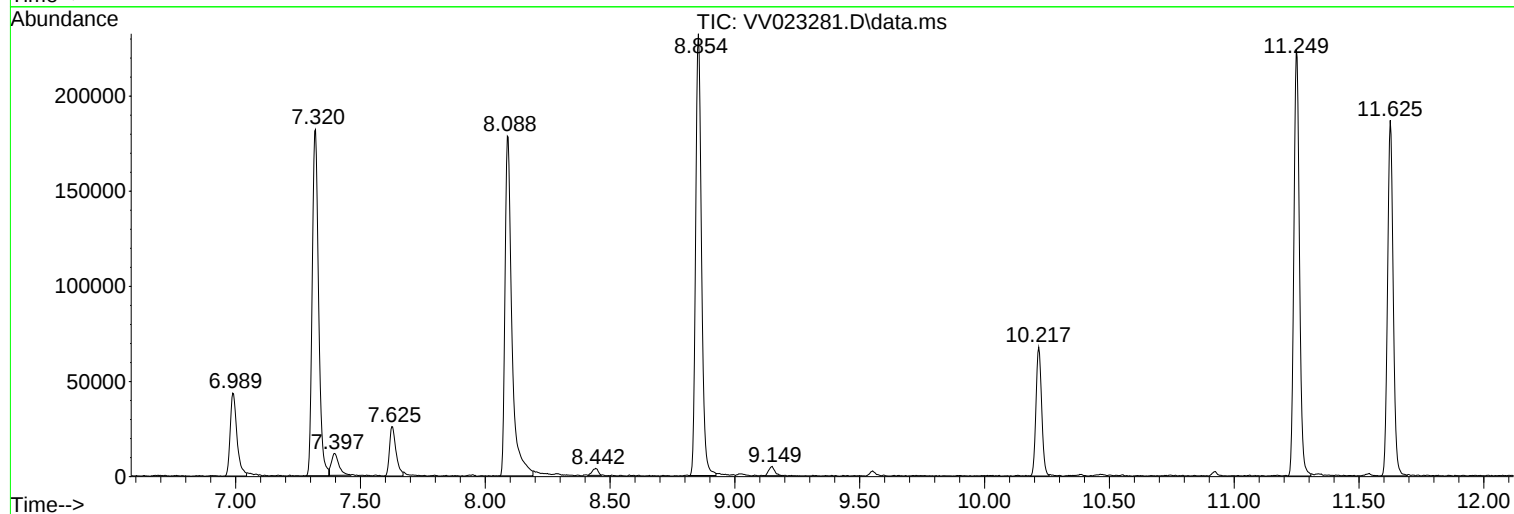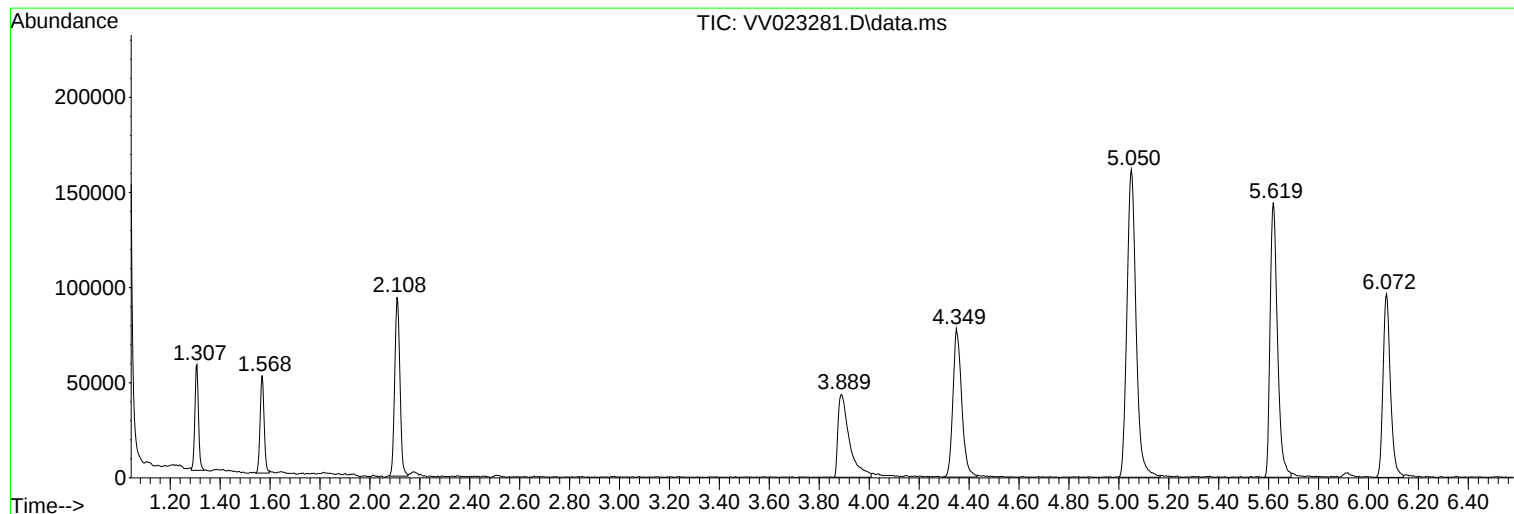

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023281.D
Acq On : 08 Nov 2021 16:10
Operator : SY/MD
Sample : M4445-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023281.D
Acq On : 08 Nov 2021 16:10
Operator : SY/MD
Sample : M4445-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
