

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
 Data File : VV023282.D
 Acq On : 08 Nov 2021 16:33
 Operator : SY/MD
 Sample : M4445-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3A6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	97	rVB	57789	60591	13.34%	1.590%
2	1.568	153	164	174	rBV	52912	60528	13.32%	1.588%
3	2.108	322	332	345	rBV	96806	142960	31.47%	3.750%
4	2.179	345	354	367	rVB2	8184	17300	3.81%	0.454%
5	3.690	811	824	834	rBV7	2078	5011	1.10%	0.131%
6	3.886	874	885	919	rBV2	48624	155862	34.31%	4.089%
7	4.349	1013	1029	1050	rBV	77838	192879	42.46%	5.060%
8	5.050	1231	1247	1280	rBV3	167354	454300	100.00%	11.918%
9	5.619	1412	1424	1444	rBV	137966	280514	61.75%	7.359%
10	5.908	1505	1514	1523	rBV3	3373	6557	1.44%	0.172%
11	6.072	1550	1565	1591	rBV	99207	210915	46.43%	5.533%
12	6.989	1837	1850	1871	rBV2	45785	87085	19.17%	2.285%
13	7.320	1941	1953	1967	rBV	191217	339198	74.66%	8.899%
14	7.394	1967	1976	1997	rVB2	36011	69650	15.33%	1.827%
15	7.625	2038	2048	2067	rBV3	27741	52282	11.51%	1.372%
16	8.088	2183	2192	2229	rBV	193022	374352	82.40%	9.821%
17	8.249	2235	2242	2259	rVB7	3815	7921	1.74%	0.208%
18	8.853	2419	2430	2450	rBV	219387	357242	78.64%	9.372%
19	9.017	2473	2481	2491	rBV4	5235	8930	1.97%	0.234%
20	9.143	2509	2520	2538	rBV2	19493	33885	7.46%	0.889%
21	9.548	2634	2646	2658	rBV	20577	32583	7.17%	0.855%
22	10.217	2839	2854	2866	rBV2	70563	109327	24.06%	2.868%
23	10.451	2917	2927	2941	rBV4	5868	10816	2.38%	0.284%
24	10.741	3009	3017	3026	rBV2	4075	5782	1.27%	0.152%
25	10.918	3062	3072	3083	rBV3	15190	23904	5.26%	0.627%
26	11.249	3165	3175	3194	rBV	220457	342944	75.49%	8.997%
27	11.342	3194	3204	3213	rVB2	7214	12884	2.84%	0.338%
28	11.532	3255	3263	3273	rBV4	10343	17753	3.91%	0.466%
29	11.625	3280	3292	3308	rBV	202514	319977	70.43%	8.394%
30	12.345	3507	3516	3527	rVB7	8530	13019	2.87%	0.342%
31	12.889	3676	3685	3691	rBV4	3534	4823	1.06%	0.127%




Sum of corrected areas: 3811774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023282.D
Acq On : 08 Nov 2021 16:33
Operator : SY/MD
Sample : M4445-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

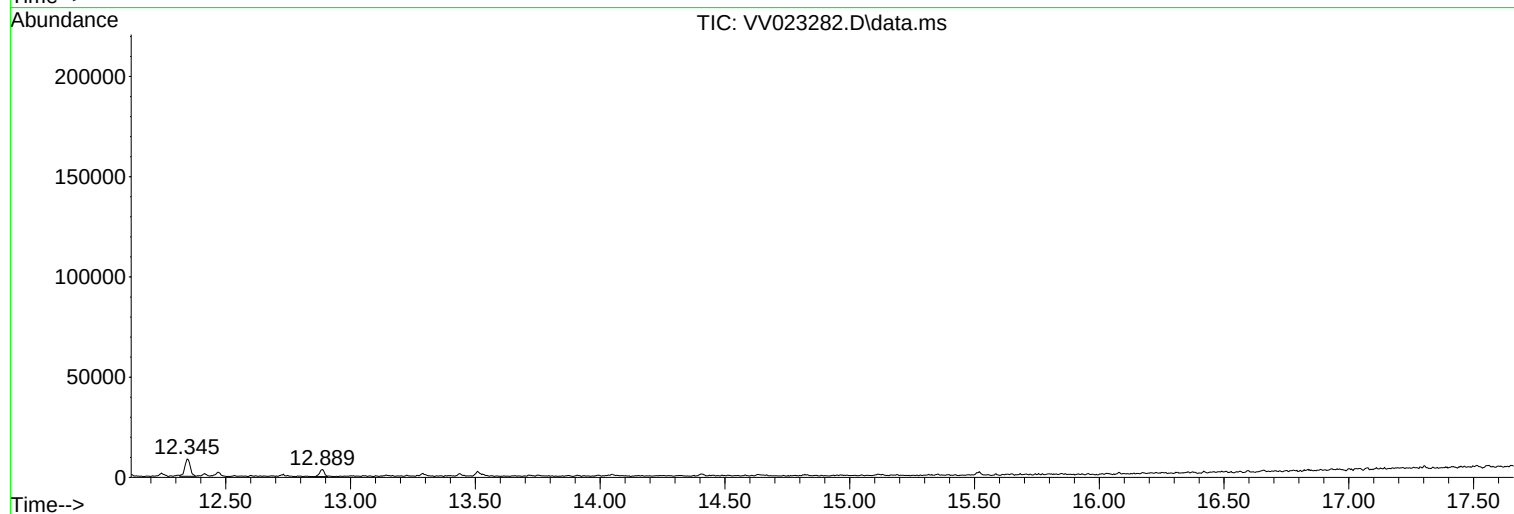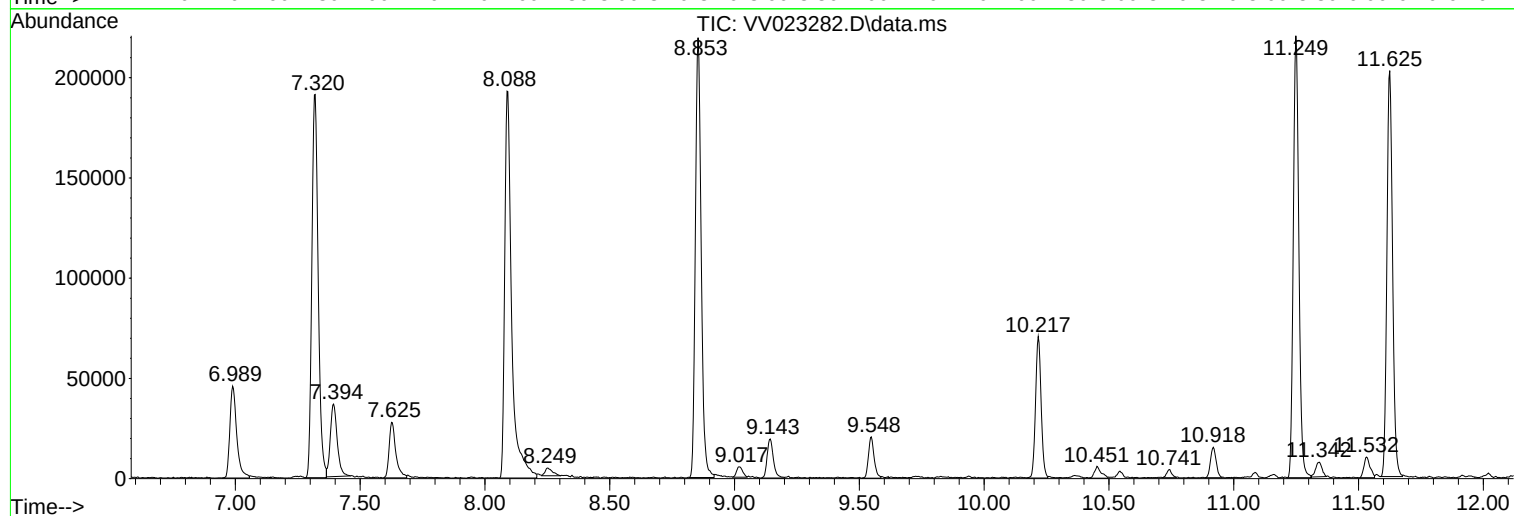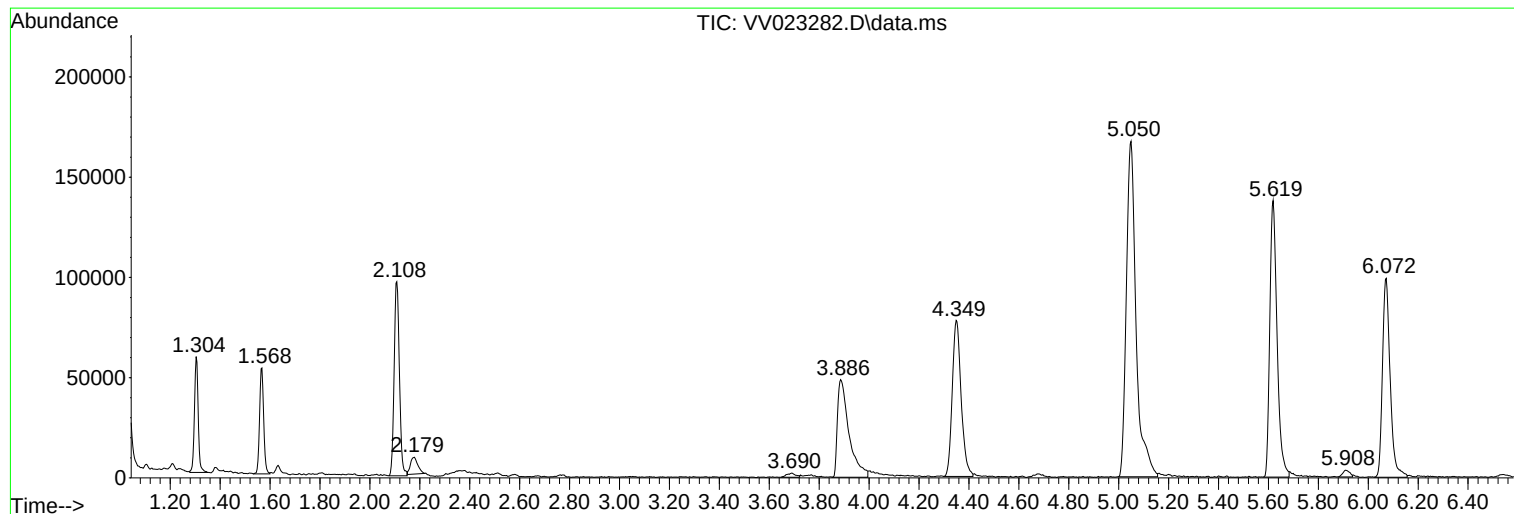

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023282.D
Acq On : 08 Nov 2021 16:33
Operator : SY/MD
Sample : M4445-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110821\
Data File : VV023282.D
Acq On : 08 Nov 2021 16:33
Operator : SY/MD
Sample : M4445-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
