

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023294.D
 Acq On : 09 Nov 2021 10:59
 Operator : SY/MD
 Sample : VV1109WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK245

Quant Time: Nov 10 00:40:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	125098	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	125938	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58901	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35023	4.469	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.568	69	31240	4.891	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	97.800%	
11) 1,1-Dichloroethene-d2	2.105	63	49827	3.396	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.000%	
20) 2-Butanone-d5	3.899	46	64840	48.024	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.040%	
24) Chloroform-d	4.349	84	81655	4.889	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.031	65	38910	5.181	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.600%	
32) Benzene-d6	5.047	84	153838	4.761	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.069	67	48771	5.127	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.600%	
41) Toluene-d8	7.317	98	127331	4.205	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.200%	
43) trans-1,3-Dichloroprop...	7.625	79	16498	4.574	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.400%	
46) 2-Hexanone-d5	8.088	63	56931	42.900	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.800%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33444	4.889	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	51074	5.208	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	8478	0.779	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023294.D
Acq On : 09 Nov 2021 10:59
Operator : SY/MD
Sample : VV1109WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245


Quant Time: Nov 10 00:40:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

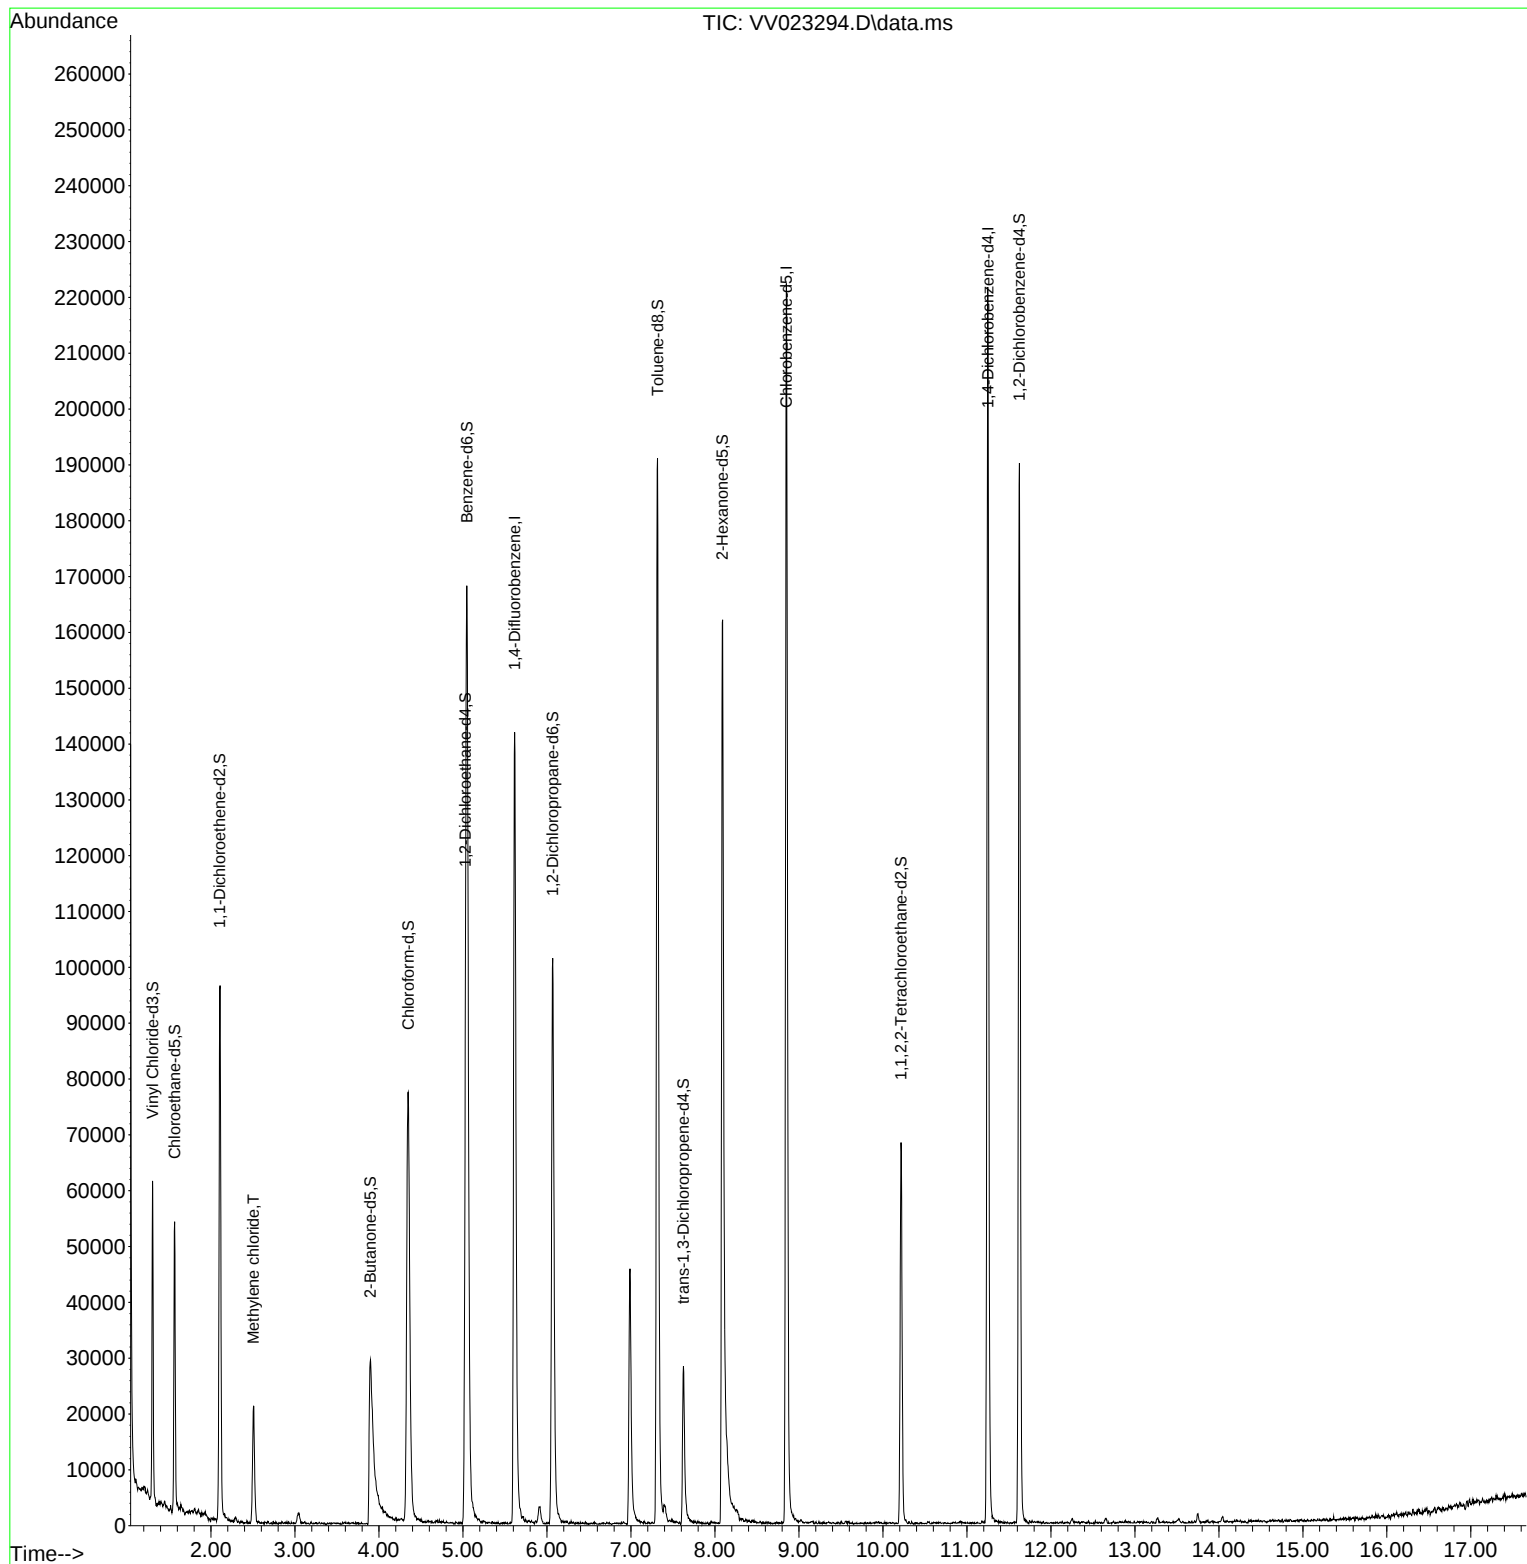

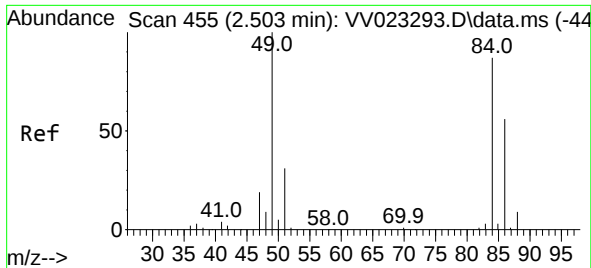

#16
Methylene chloride
Concen: 0.779 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV023294.D
Acq: 09 Nov 2021 10:59

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

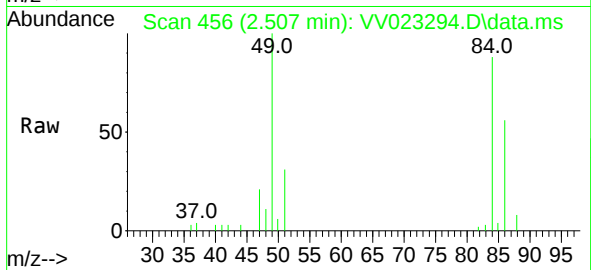

Tgt Ion: 84 Resp: 8478

Ion	Ratio	Lower	Upper
84	100		
86	63.3	42.3	78.5
49	113.8	79.7	148.1

