

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110921\
 Data File : VW023303.D
 Acq On : 09 Nov 2021 15:13
 Operator : SY/MD
 Sample : M4558-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB883

Quant Time: Nov 10 00:42:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	132073	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	134356	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61833	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	34987	4.229	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.600%
7) Chloroethane-d5	1.568	69	32259	4.784	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.108	63	51648	3.334	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.600%
20) 2-Butanone-d5	3.886	46	89721	62.943	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.880%
24) Chloroform-d	4.349	84	82329	4.669	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	5.034	65	38645	4.874	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%
32) Benzene-d6	5.050	84	153299	4.447	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.069	67	47863	4.717	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.400%
41) Toluene-d8	7.317	98	126273	3.909	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.200%
43) trans-1,3-Dichloroprop...	7.625	79	15456	4.017	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.088	63	61448	43.403	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.800%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30159	4.133	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	50530	4.908	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.200%
Target Compounds					Qvalue	
13) Acetone	2.175	43	13256	15.220	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023303.D
Acq On : 09 Nov 2021 15:13
Operator : SY/MD
Sample : M4558-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB883

Quant Time: Nov 10 00:42:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

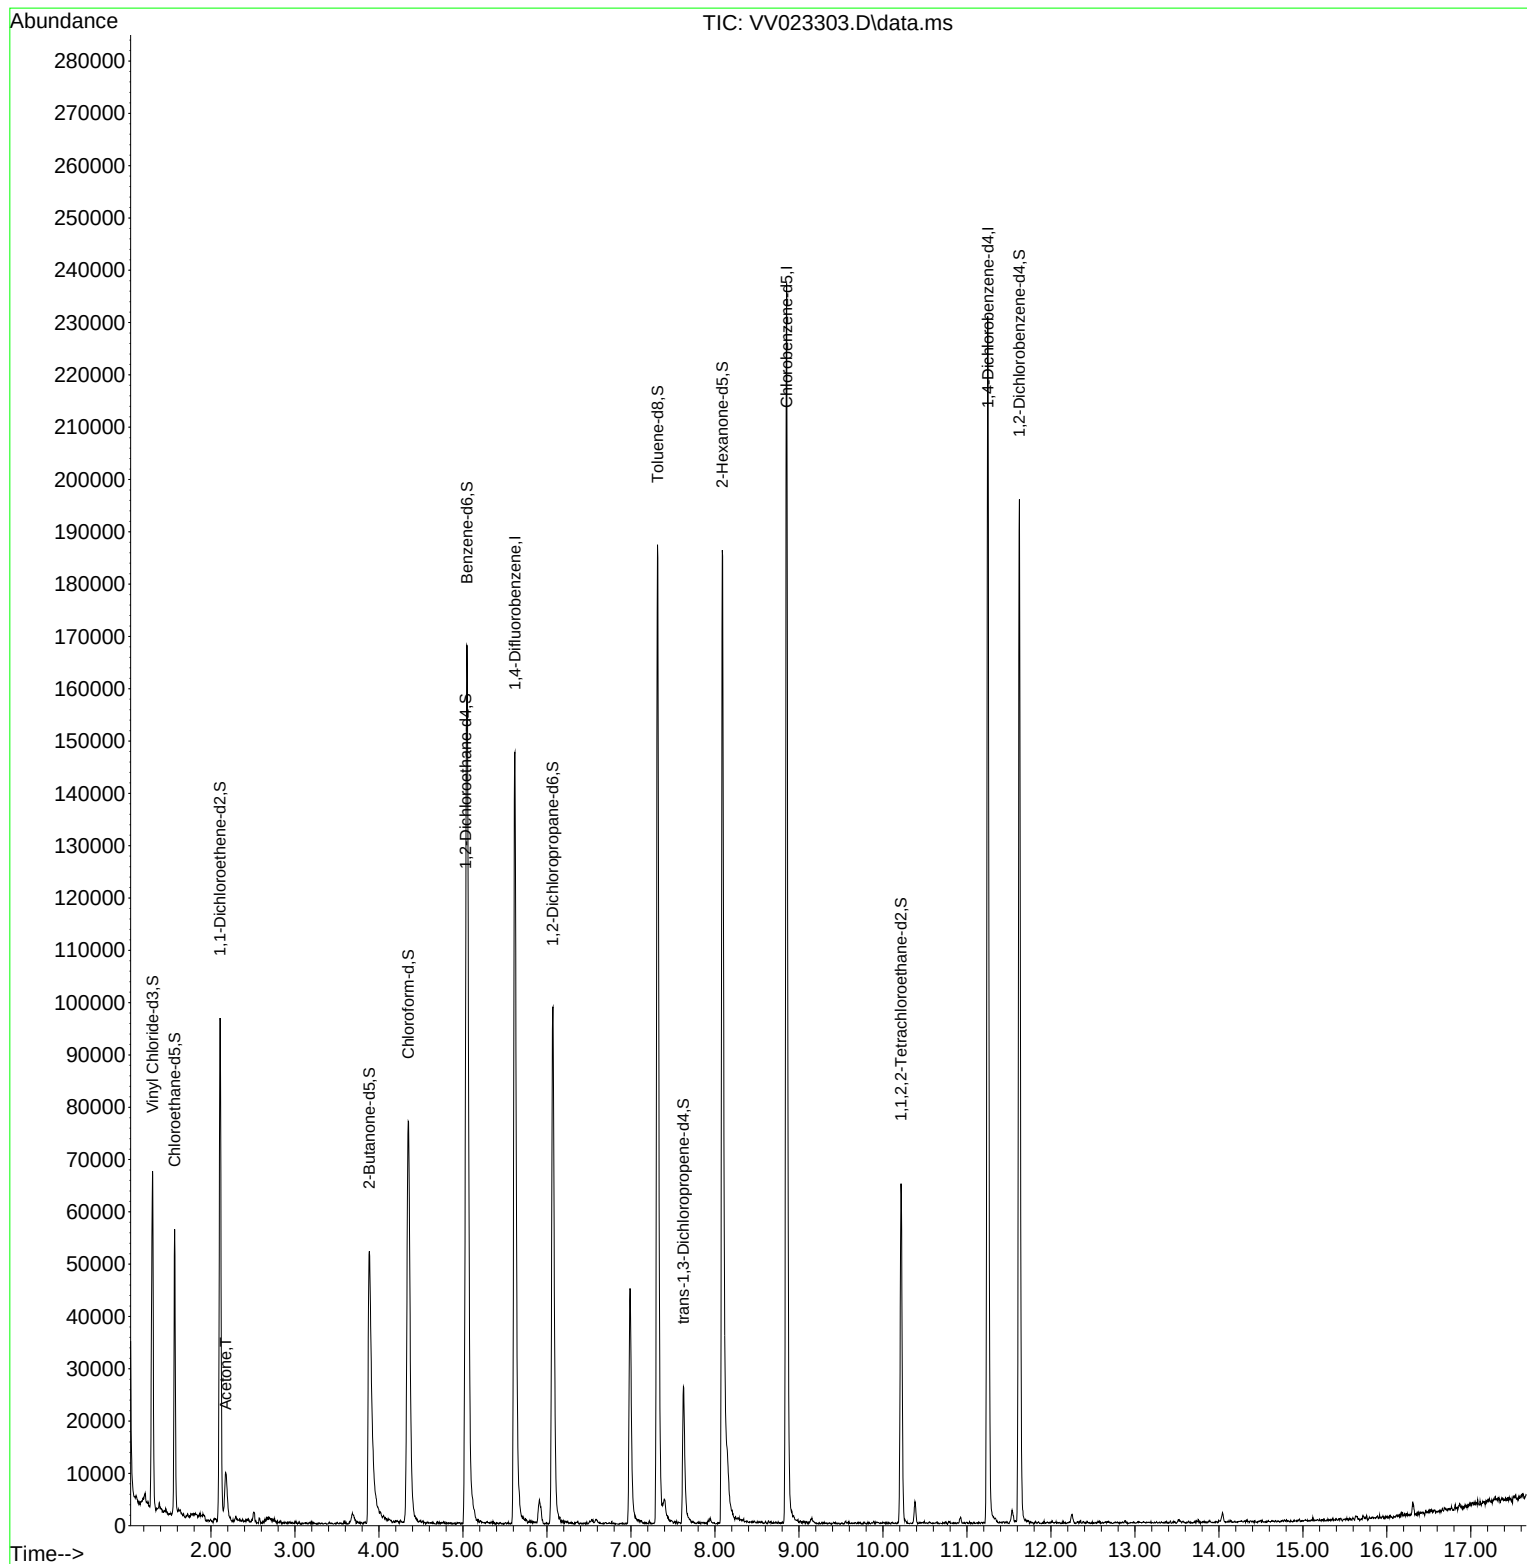

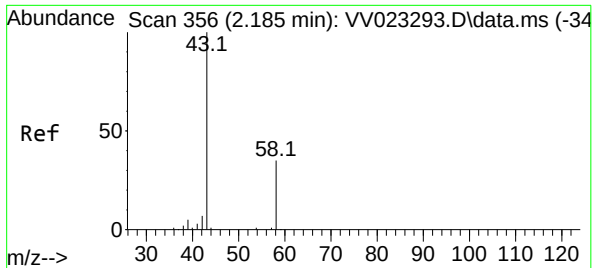

#13
 Acetone
 Concen: 15.220 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV023303.D
 Acq: 09 Nov 2021 15:13

Instrument :
 MSVOA_V
 ClientSampleId :
 GB883

Tgt Ion: 43 Resp: 13256
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 55.4

