

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110921\
 Data File : VW023304.D
 Acq On : 09 Nov 2021 15:36
 Operator : SY/MD
 Sample : M4558-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB884

Quant Time: Nov 10 00:43:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	130908	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	131123	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61849	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	33777	4.119	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.400%
7) Chloroethane-d5	1.568	69	31813	4.760	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.111	63	49426	3.219	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.400%
20) 2-Butanone-d5	3.889	46	88747	62.813	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.620%
24) Chloroform-d	4.352	84	79740	4.562	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.037	65	37887	4.821	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.400%
32) Benzene-d6	5.053	84	150643	4.478	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	6.072	67	47566	4.803	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.320	98	124444	3.947	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
43) trans-1,3-Dichloroprop...	7.625	79	16417	4.372	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.400%
46) 2-Hexanone-d5	8.088	63	59645	43.168	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.340%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30757	4.318	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	49983	4.853	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	2737	3.170	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023304.D
Acq On : 09 Nov 2021 15:36
Operator : SY/MD
Sample : M4558-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB884

Quant Time: Nov 10 00:43:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

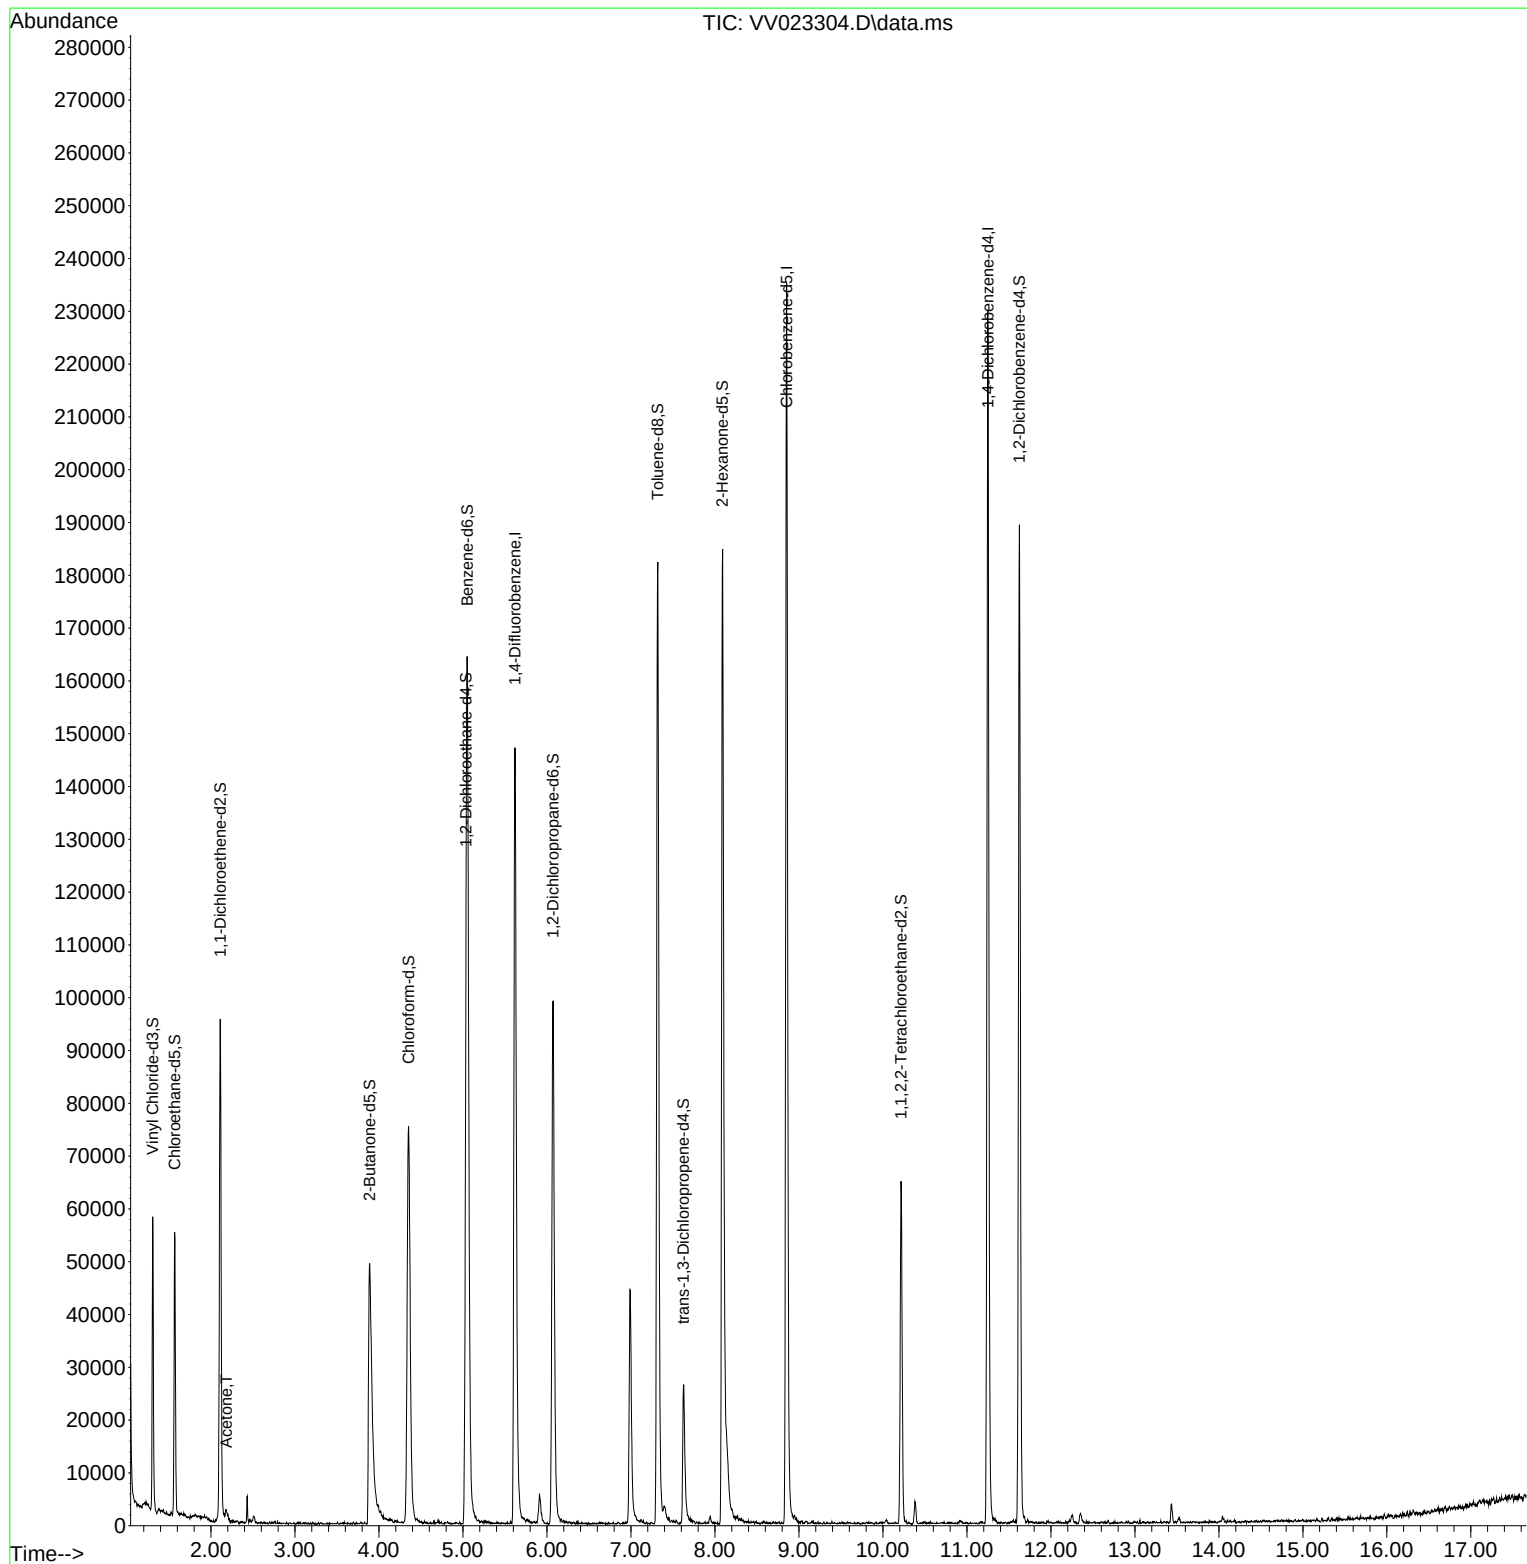

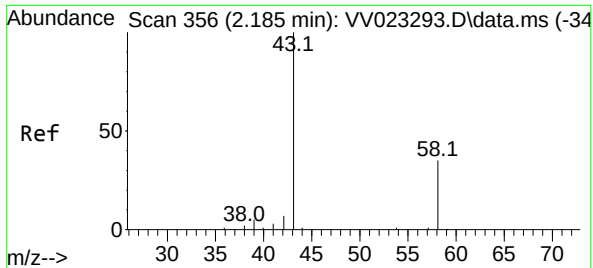

#13
 Acetone
 Concen: 3.170 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV023304.D
 Acq: 09 Nov 2021 15:36

Instrument :
 MSVOA_V
 ClientSampleId :
 GB884

Tgt Ion: 43 Resp: 2737

Ion	Ratio	Lower	Upper
43	100		
58	33.4	0.0	55.4

