

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW110921\  
 Data File : VW023306.D  
 Acq On : 09 Nov 2021 16:23  
 Operator : SY/MD  
 Sample : M4558-24  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 GB886

Quant Time: Nov 10 00:43:29 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 10 00:38:37 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|----------|----------|
| -----                         |        |                |          |        |          |          |
| Internal Standards            |        |                |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114            | 142531   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.854  | 117            | 144287   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152            | 67064    | 5.000  | ug/L     | 0.00     |
|                               |        |                |          |        |          |          |
| System Monitoring Compounds   |        |                |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65             | 31837    | 3.566  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 71.400%  |          |
| 7) Chloroethane-d5            | 1.568  | 69             | 29633    | 4.072  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 81.400%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.111  | 63             | 47552    | 2.845  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 56.800%# |          |
| 20) 2-Butanone-d5             | 3.892  | 46             | 89278    | 58.036 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 116.080% |          |
| 24) Chloroform-d              | 4.352  | 84             | 78475    | 4.124  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 82.400%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.034  | 65             | 37667    | 4.402  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 88.000%  |          |
| 32) Benzene-d6                | 5.053  | 84             | 145463   | 3.929  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 78.600%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.072  | 67             | 47293    | 4.340  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 86.800%  |          |
| 41) Toluene-d8                | 7.317  | 98             | 118467   | 3.415  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 68.200%# |          |
| 43) trans-1,3-Dichloroprop... | 7.628  | 79             | 15695    | 3.798  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 76.000%  |          |
| 46) 2-Hexanone-d5             | 8.091  | 63             | 60674    | 39.907 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 79.820%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84             | 30376    | 3.876  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 77.600%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152            | 49270    | 4.412  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 88.200%  |          |
|                               |        |                |          |        |          |          |
| Target Compounds              |        |                |          |        | Qvalue   |          |
| 13) Acetone                   | 2.182  | 43             | 36097    | 38.403 | ug/L     | 92       |
| -----                         |        |                |          |        |          |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110921\  
Data File : VV023306.D  
Acq On : 09 Nov 2021 16:23  
Operator : SY/MD  
Sample : M4558-24  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
GB886

Quant Time: Nov 10 00:43:29 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 10 00:38:37 2021  
Response via : Initial Calibration

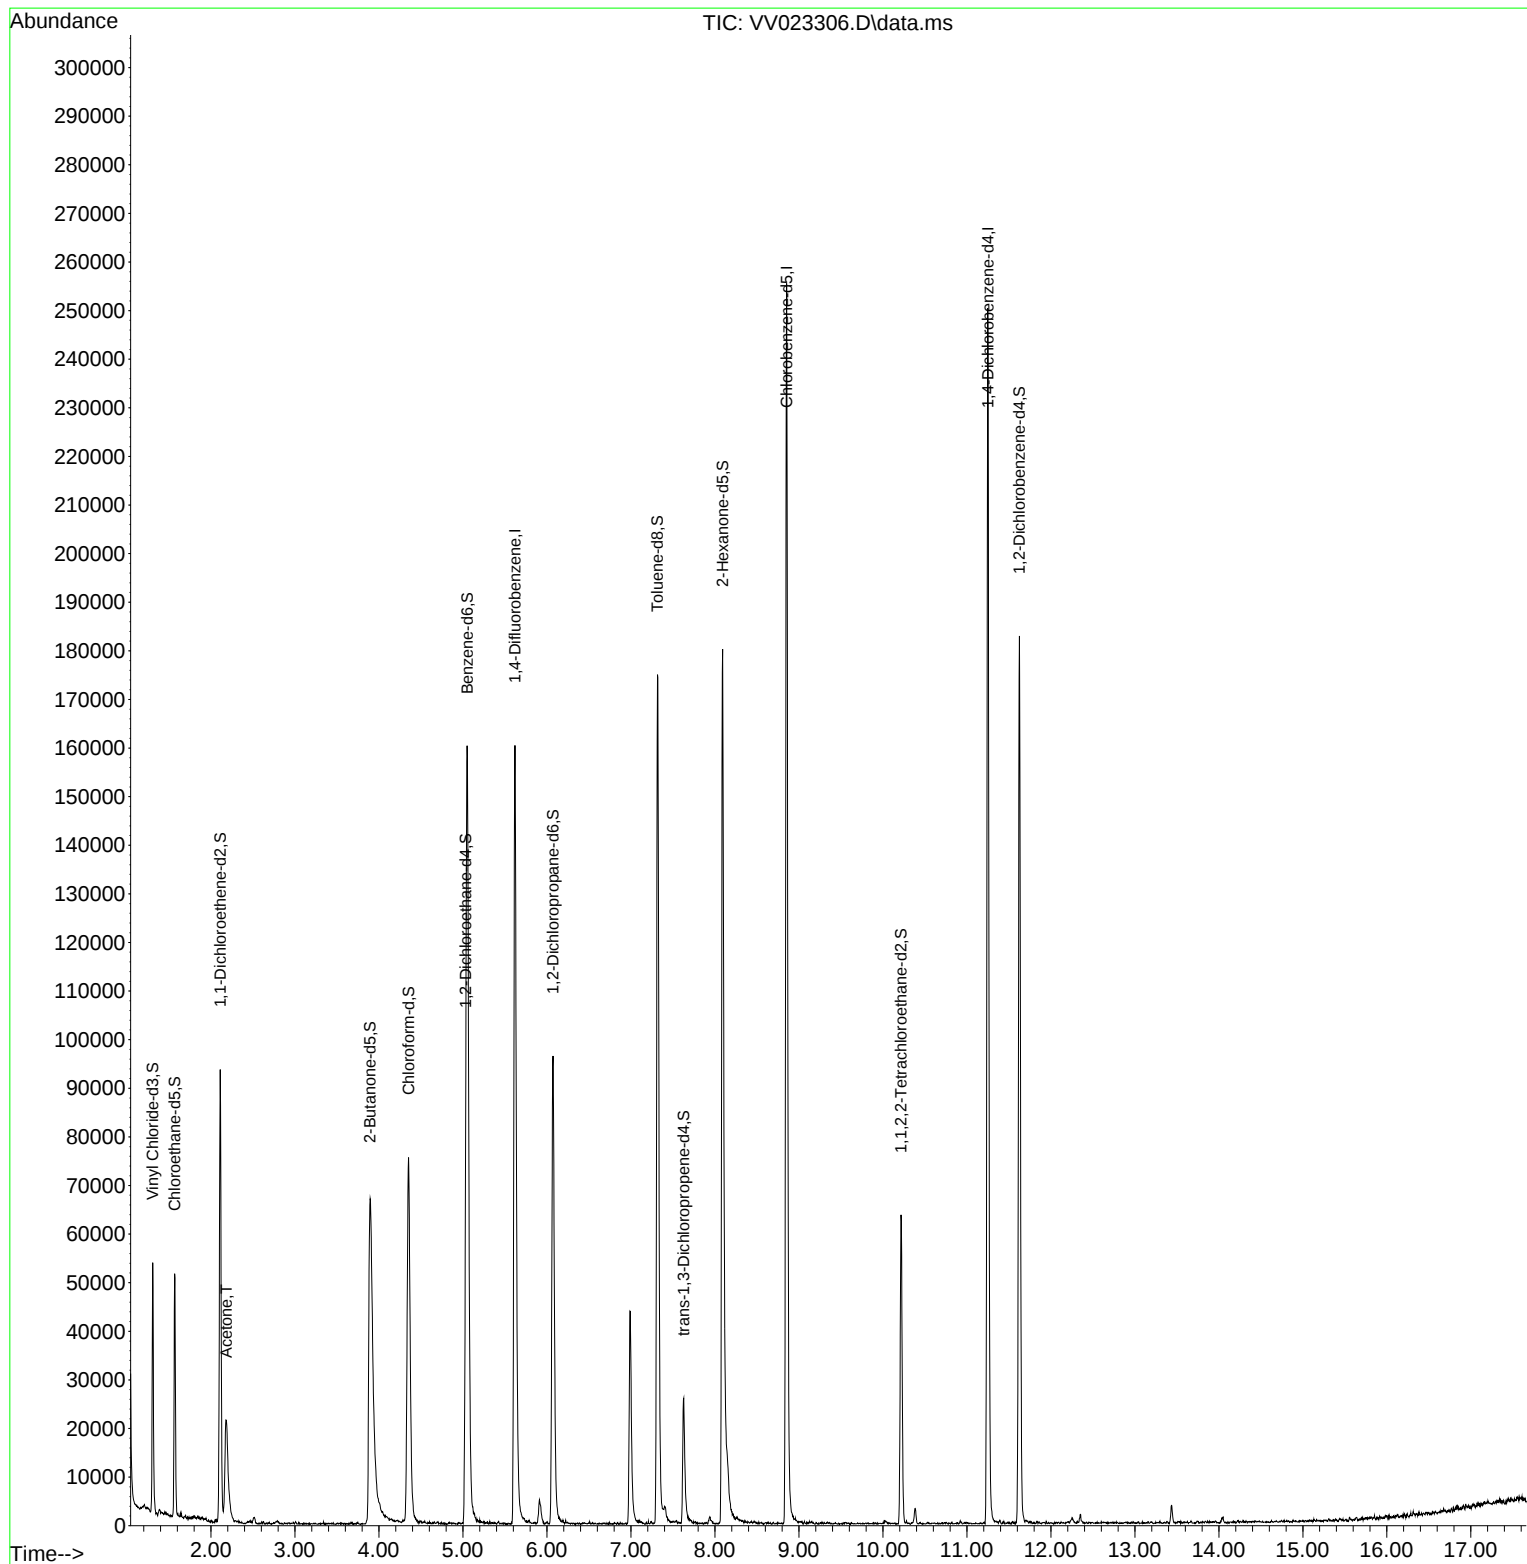

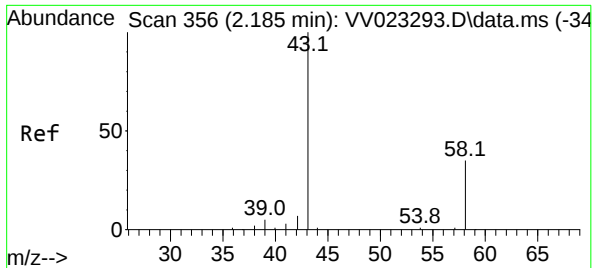

#13  
 Acetone  
 Concen: 38.403 ug/L  
 RT: 2.182 min Scan# 31  
 Delta R.T. -0.003 min  
 Lab File: VV023306.D  
 Acq: 09 Nov 2021 16:23

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 GB886

Tgt Ion: 43 Resp: 36097  
 Ion Ratio Lower Upper  
 43 100  
 58 31.9 0.0 55.4

