

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110921\
 Data File : VW023312.D
 Acq On : 09 Nov 2021 18:43
 Operator : SY/MD
 Sample : M4522-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG396

Quant Time: Nov 10 00:44:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	124451	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	124752	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58559	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	30491	3.911	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%
7) Chloroethane-d5	1.568	69	28779	4.529	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.111	63	44746	3.066	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.400%
20) 2-Butanone-d5	3.889	46	90524	67.395	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.800%#
24) Chloroform-d	4.352	84	78510	4.725	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.037	65	38023	5.089	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%
32) Benzene-d6	5.053	84	141503	4.421	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
36) 1,2-Dichloropropane-d6	6.072	67	46626	4.948	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.317	98	119385	3.980	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	7.625	79	15555	4.354	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.088	63	63006	47.930	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.860%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33581	4.956	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	49382	5.064	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds						Qvalue
13) Acetone	2.185	43	2219	2.704	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023312.D
Acq On : 09 Nov 2021 18:43
Operator : SY/MD
Sample : M4522-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG396

Quant Time: Nov 10 00:44:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

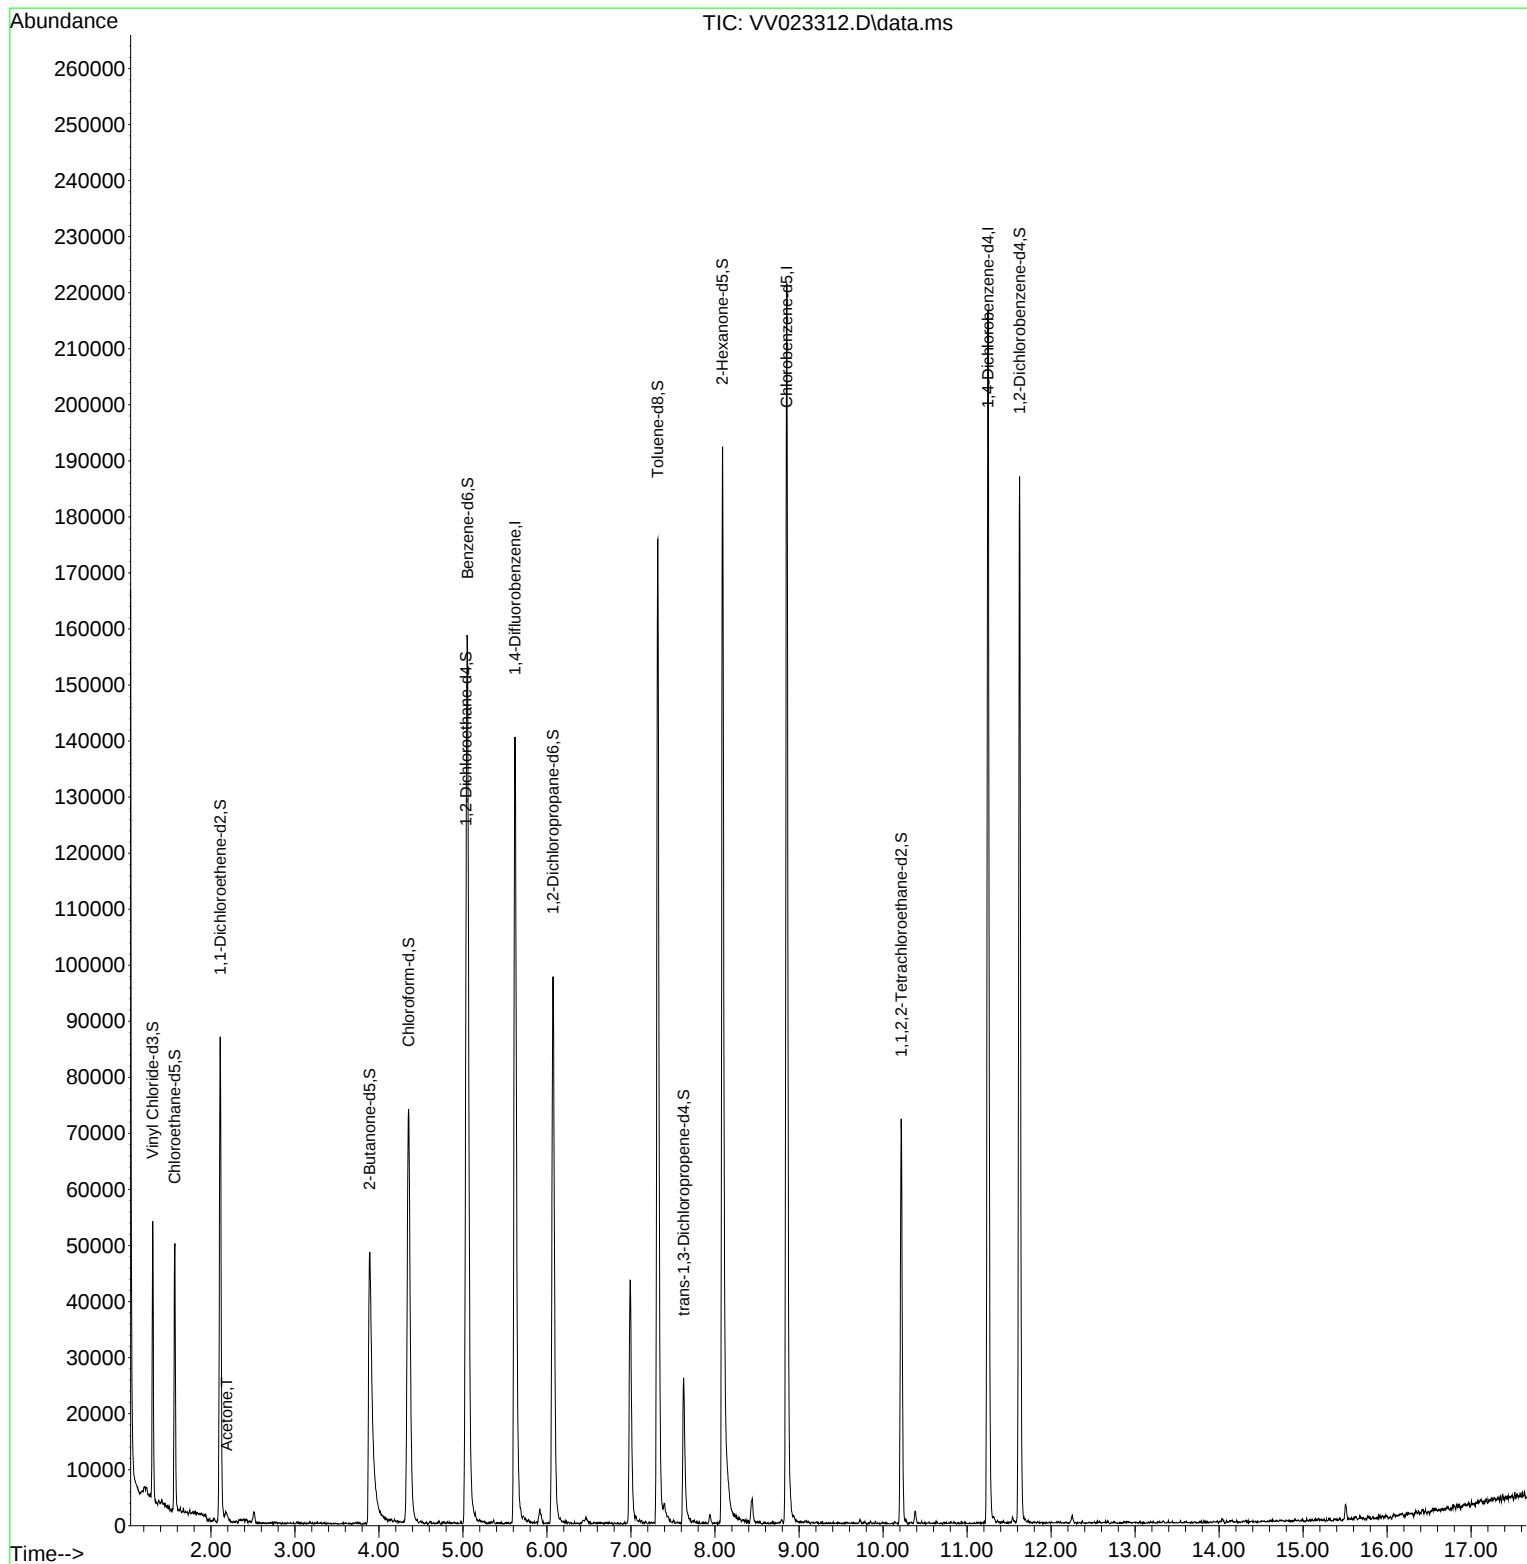

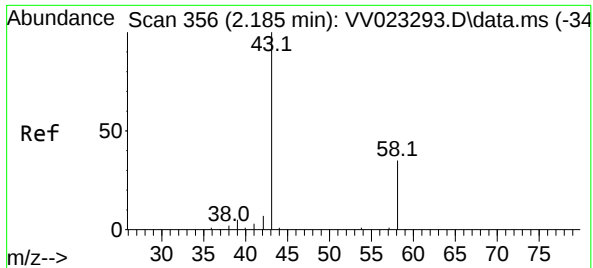

#13
 Acetone
 Concen: 2.704 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV023312.D
 Acq: 09 Nov 2021 18:43

Instrument :
 MSVOA_V
 ClientSampleId :
 BG396

Tgt Ion: 43 Resp: 2219
 Ion Ratio Lower Upper
 43 100
 58 27.2 0.0 55.4

