

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023313.D
 Acq On : 09 Nov 2021 19:07
 Operator : SY/MD
 Sample : M4522-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG397

Quant Time: Nov 10 00:45:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123369	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126022	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56934	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	28067	3.632	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.568	69	26956	4.279	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.111	63	41174	2.846	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.000%#
20) 2-Butanone-d5	3.889	46	82286	61.800	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.600%
24) Chloroform-d	4.352	84	72701	4.414	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%
26) 1,2-Dichloroethane-d4	5.034	65	36091	4.873	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%
32) Benzene-d6	5.053	84	133839	4.139	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
36) 1,2-Dichloropropane-d6	6.072	67	43264	4.545	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.000%
41) Toluene-d8	7.320	98	109808	3.624	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
43) trans-1,3-Dichloroprop...	7.629	79	14710	4.076	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.600%
46) 2-Hexanone-d5	8.088	63	58757	44.247	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.500%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31487	4.600	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	47296	4.989	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds					Qvalue	
13) Acetone	2.175	43	3462	4.255	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023313.D
Acq On : 09 Nov 2021 19:07
Operator : SY/MD
Sample : M4522-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG397

Quant Time: Nov 10 00:45:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

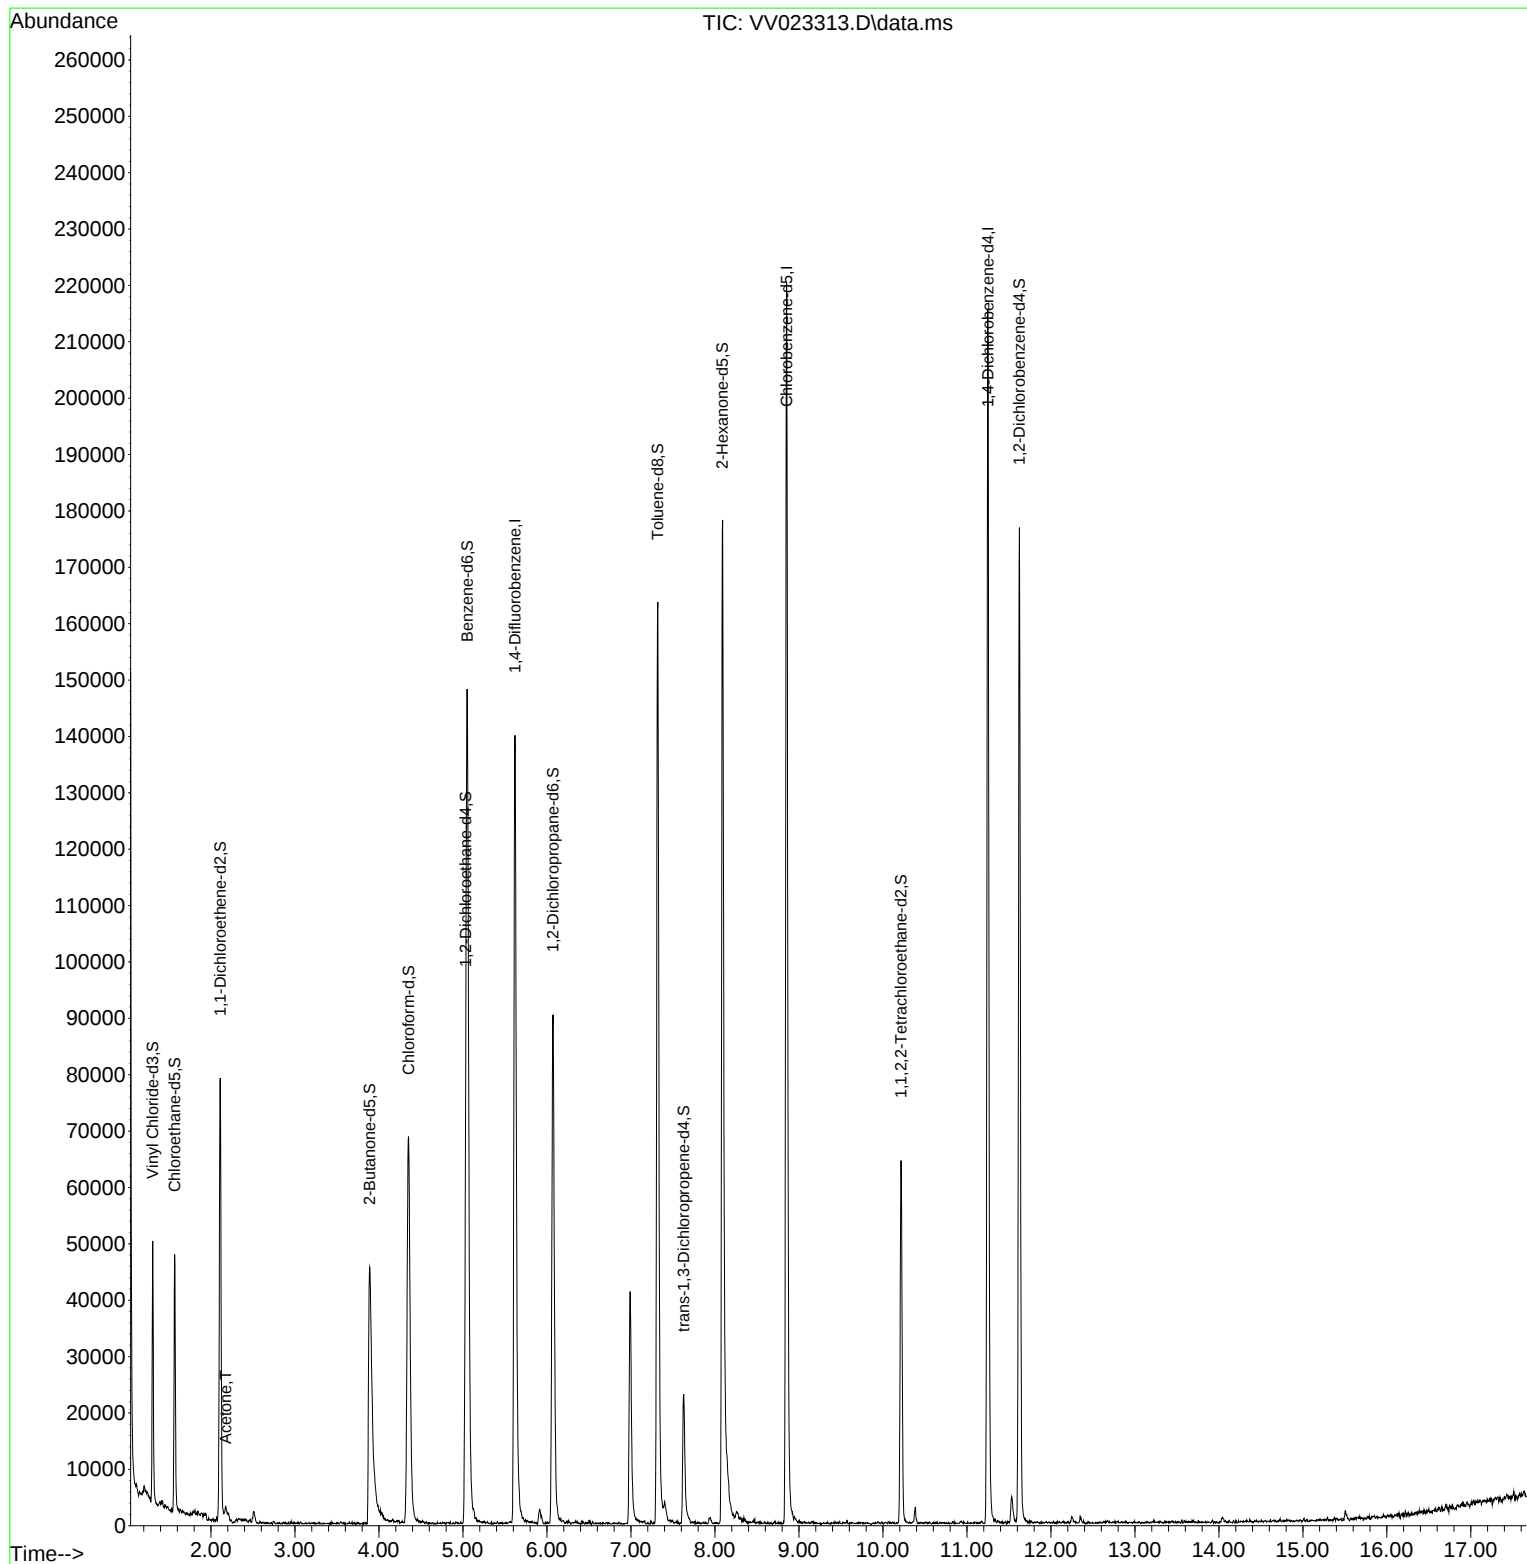

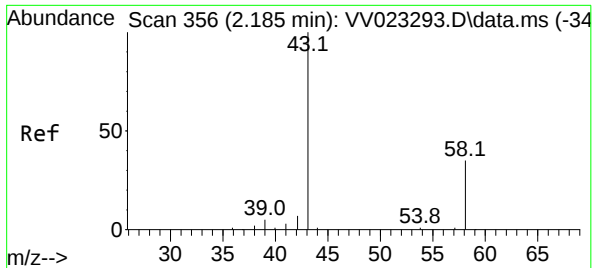

#13
 Acetone
 Concen: 4.255 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV023313.D
 Acq: 09 Nov 2021 19:07

Instrument :
 MSVOA_V
 ClientSampleId :
 BG397

Tgt Ion: 43 Resp: 3462
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 55.4

