

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023314.D
 Acq On : 09 Nov 2021 19:30
 Operator : SY/MD
 Sample : M4522-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG398

Quant Time: Nov 10 00:45:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117430	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	117594	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54378	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	28403	3.861	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.200%
7) Chloroethane-d5	1.568	69	26695	4.452	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	2.108	63	42000	3.050	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.000%
20) 2-Butanone-d5	3.886	46	83160	65.615	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.220%#
24) Chloroform-d	4.352	84	74207	4.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.037	65	35176	4.989	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	5.053	84	136777	4.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.072	67	43966	4.950	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.320	98	111947	3.959	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.200%
43) trans-1,3-Dichloroprop...	7.629	79	15159	4.501	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.088	63	57602	46.486	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.980%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30624	4.794	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	45530	5.028	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%
Target Compounds					Qvalue	
13) Acetone	2.172	43	2522	3.257	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023314.D
Acq On : 09 Nov 2021 19:30
Operator : SY/MD
Sample : M4522-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG398

Quant Time: Nov 10 00:45:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

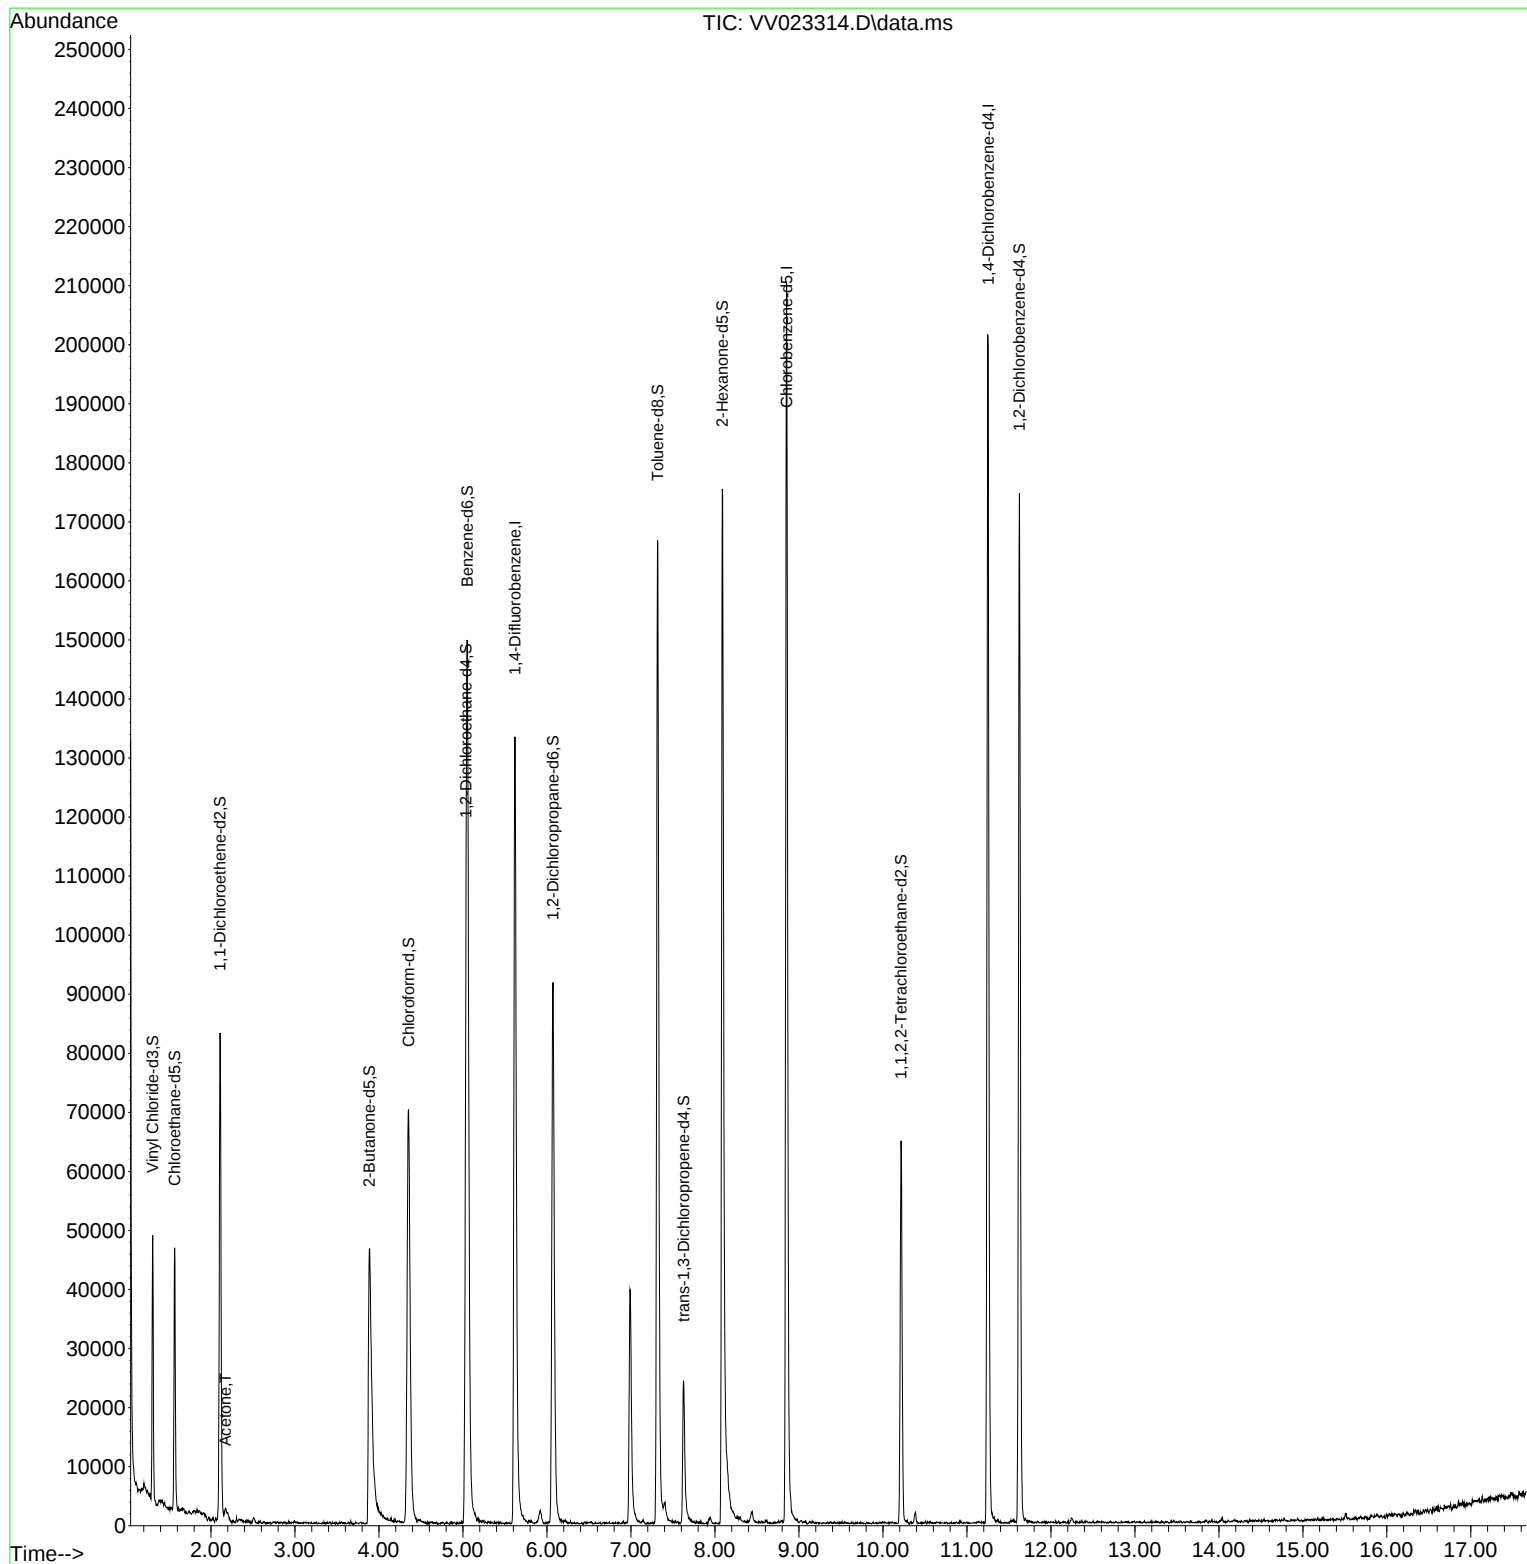

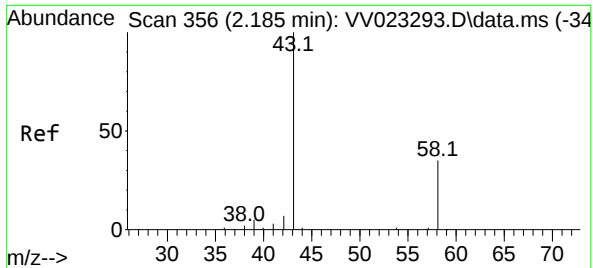

#13
 Acetone
 Concen: 3.257 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV023314.D
 Acq: 09 Nov 2021 19:30

Instrument :
 MSVOA_V
 ClientSampleId :
 BG398

Tgt Ion: 43 Resp: 2522

Ion	Ratio	Lower	Upper
43	100		
58	29.2	0.0	55.4

