

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110921\
 Data File : VW023315.D
 Acq On : 09 Nov 2021 19:54
 Operator : SY/MD
 Sample : M4522-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG399

Quant Time: Nov 10 00:45:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	119403	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	120846	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	56809	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	27710	3.704	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	74.000%	
7) Chloroethane-d5	1.568	69	25947	4.256	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.200%	
11) 1,1-Dichloroethene-d2	2.108	63	41099	2.935	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.600%#	
20) 2-Butanone-d5	3.886	46	83716	64.962	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	129.920%	
24) Chloroform-d	4.352	84	73434	4.607	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
26) 1,2-Dichloroethane-d4	5.037	65	34937	4.874	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.400%	
32) Benzene-d6	5.053	84	132998	4.289	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.800%	
36) 1,2-Dichloropropane-d6	6.072	67	42749	4.684	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.600%	
41) Toluene-d8	7.320	98	110107	3.789	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	75.800%	
43) trans-1,3-Dichloroprop...	7.628	79	14451	4.175	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.600%	
46) 2-Hexanone-d5	8.088	63	57419	45.091	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.180%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30560	4.656	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	45632	4.824	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.400%	
Target Compounds					Qvalue	
13) Acetone	2.175	43	2317	2.942	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023315.D
Acq On : 09 Nov 2021 19:54
Operator : SY/MD
Sample : M4522-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG399

Quant Time: Nov 10 00:45:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 10 00:38:37 2021
Response via : Initial Calibration

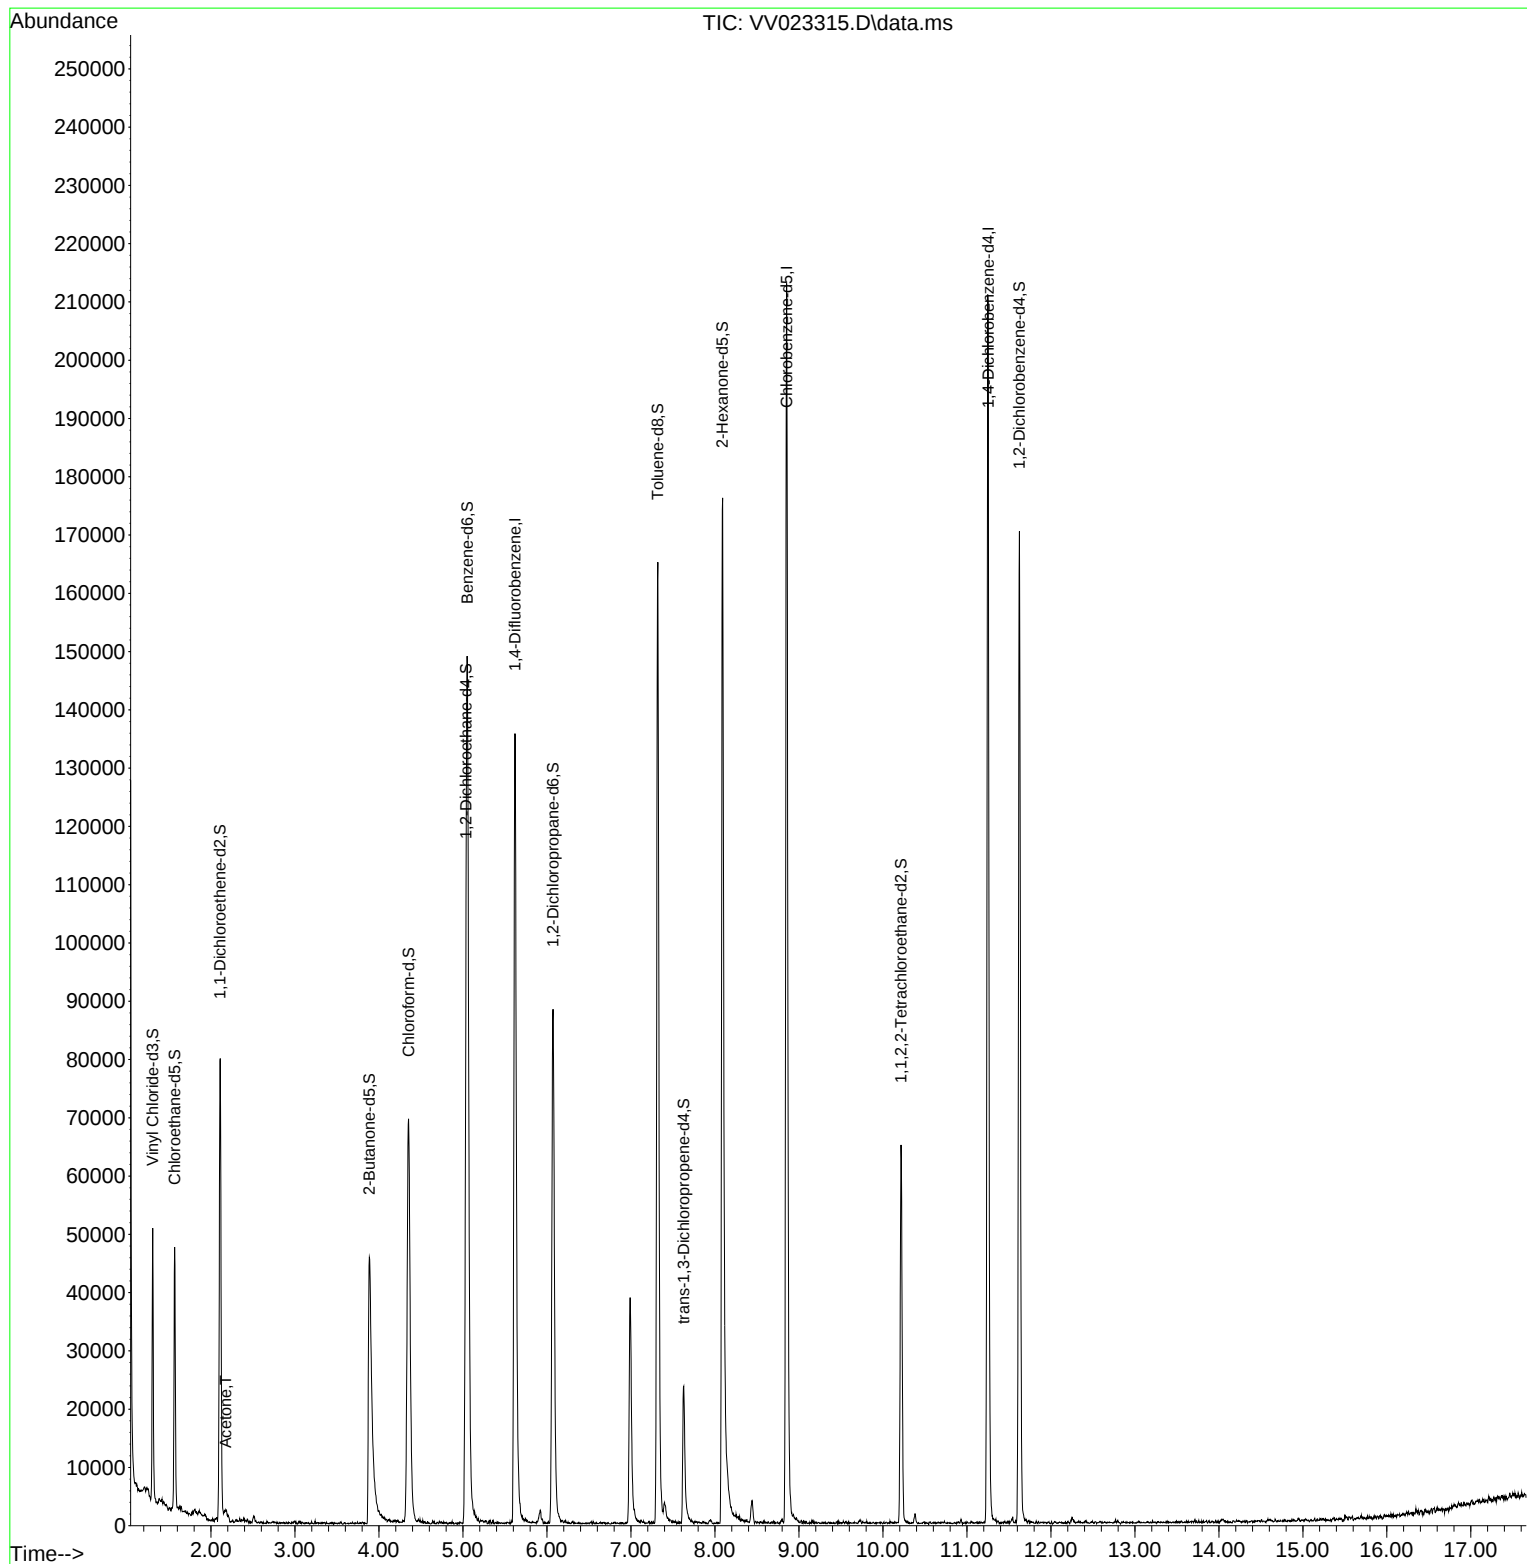

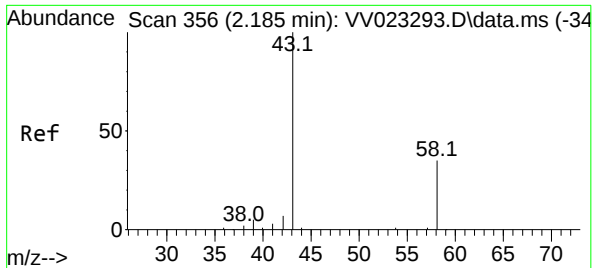

#13
 Acetone
 Concen: 2.942 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV023315.D
 Acq: 09 Nov 2021 19:54

Instrument :
 MSVOA_V
 ClientSampleId :
 BG399

Tgt Ion: 43 Resp: 2317
 Ion Ratio Lower Upper
 43 100
 58 29.5 0.0 55.4

