

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023324.D
 Acq On : 10 Nov 2021 11:50
 Operator : SY/MD
 Sample : M4522-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 11 00:40:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 11 00:38:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123679	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	125554	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57507	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	30016	3.874	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.400%	
7) Chloroethane-d5	1.568	69	28355	4.490	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.800%	
11) 1,1-Dichloroethene-d2	2.111	63	43829	3.022	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.400%	
20) 2-Butanone-d5	3.889	46	85281	63.888	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	127.780%	
24) Chloroform-d	4.352	84	76638	4.641	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.800%	
26) 1,2-Dichloroethane-d4	5.037	65	37228	5.014	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.053	84	138492	4.299	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.000%	
36) 1,2-Dichloropropane-d6	6.072	67	45850	4.835	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.600%	
41) Toluene-d8	7.320	98	115082	3.812	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.200%	
43) trans-1,3-Dichloroprop...	7.628	79	14247	3.962	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.200%	
46) 2-Hexanone-d5	8.088	63	59835	45.227	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.460%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32814	4.812	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	47610	4.972	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.400%	
Target Compounds					Qvalue	
13) Acetone	2.175	43	1234	1.513	ug/L	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023324.D
Acq On : 10 Nov 2021 11:50
Operator : SY/MD
Sample : M4522-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 11 00:40:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 11 00:38:57 2021
Response via : Initial Calibration

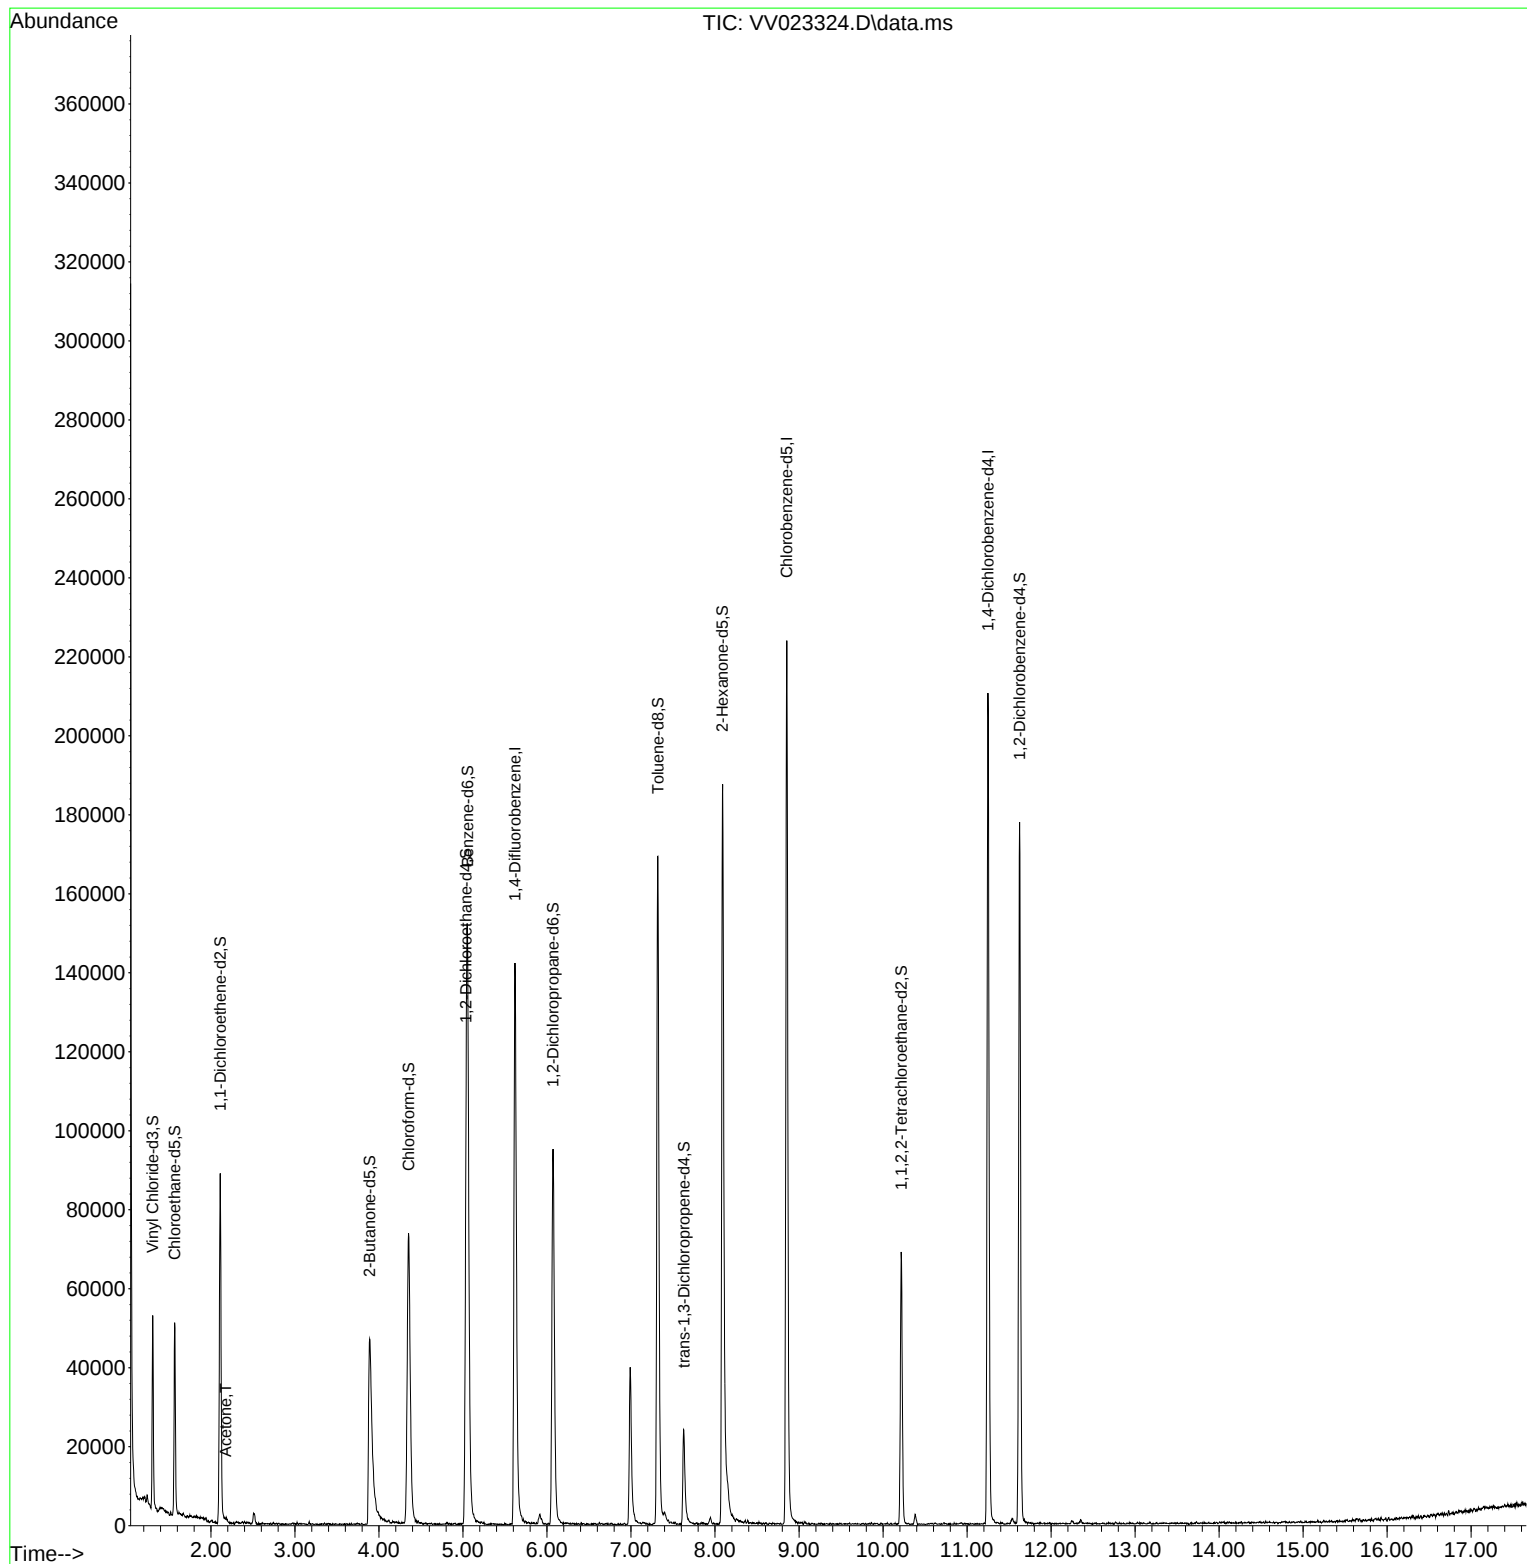

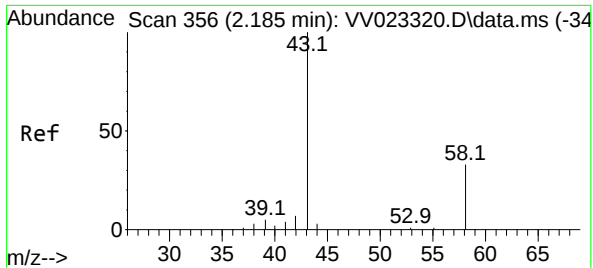

#13
 Acetone
 Concen: 1.513 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV023324.D
 Acq: 10 Nov 2021 11:50

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

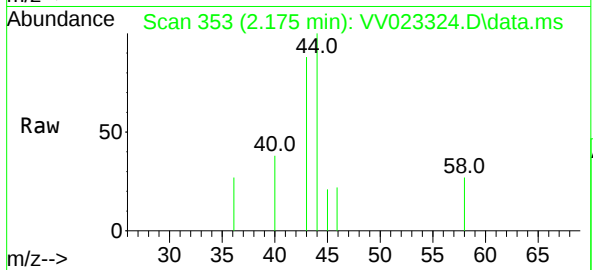

Tgt Ion: 43 Resp: 1234
 Ion Ratio Lower Upper
 43 100
 58 11.7 0.0 55.4

