

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023328.D
 Acq On : 10 Nov 2021 13:22
 Operator : SY/MD
 Sample : M4545-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 11 00:41:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 11 00:38:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123922	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	127578	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57892	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	40447	5.210	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.200%
7) Chloroethane-d5	1.568	69	33060	5.225	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.600%
11) 1,1-Dichloroethene-d2	2.108	63	55465	3.816	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.400%
20) 2-Butanone-d5	3.902	46	69303	51.817	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.640%
24) Chloroform-d	4.352	84	72963	4.410	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%
26) 1,2-Dichloroethane-d4	5.037	65	34555	4.645	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.053	84	145136	4.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
36) 1,2-Dichloropropane-d6	6.072	67	44433	4.611	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.200%
41) Toluene-d8	7.320	98	124577	4.061	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.200%
43) trans-1,3-Dichloroprop...	7.628	79	15192	4.158	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.200%
46) 2-Hexanone-d5	8.091	63	50003	37.195	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.400%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27473	3.965	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	47388	4.916	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.400%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.510	84	4408	0.409	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023328.D
Acq On : 10 Nov 2021 13:22
Operator : SY/MD
Sample : M4545-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Nov 11 00:41:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 11 00:38:57 2021
Response via : Initial Calibration

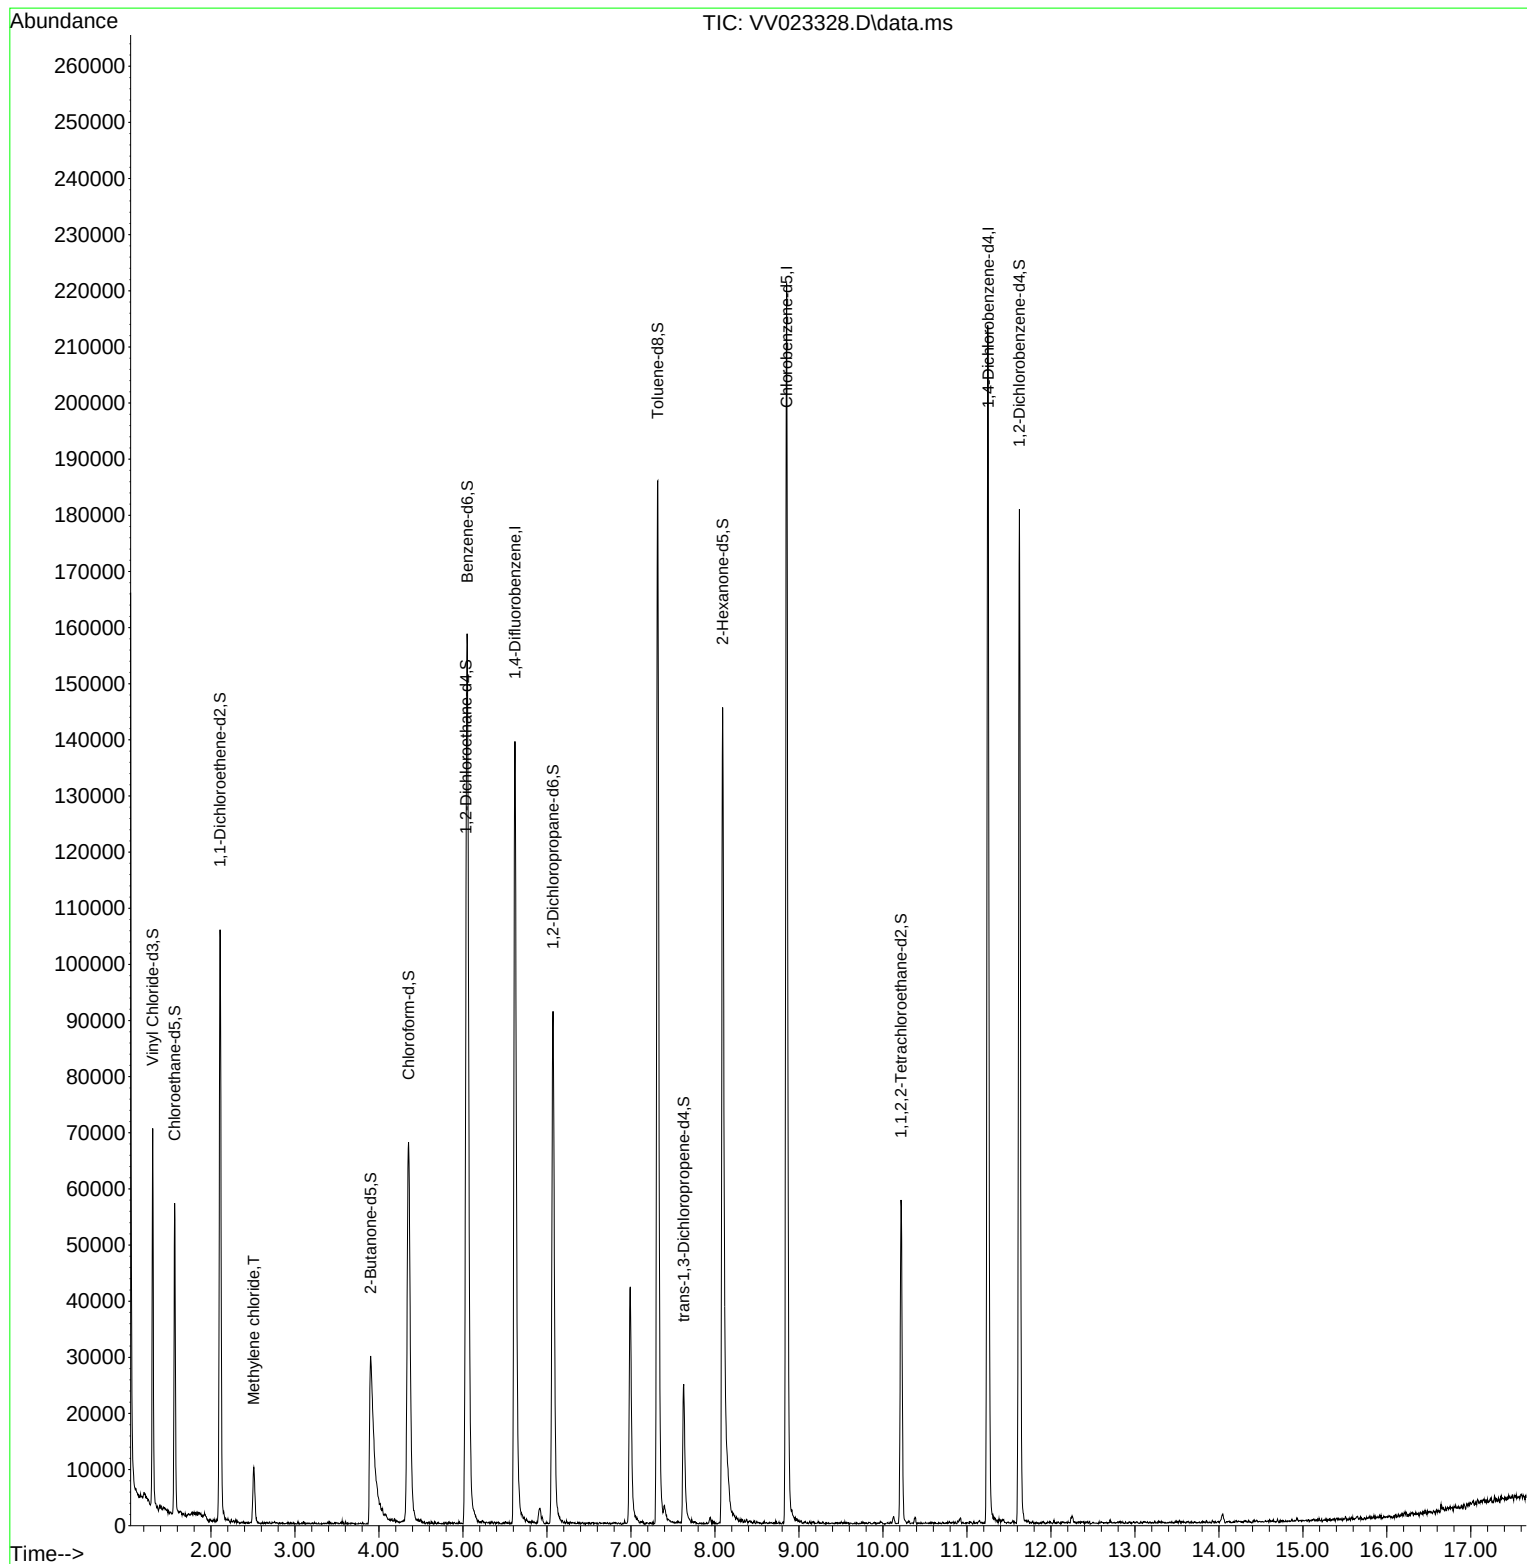

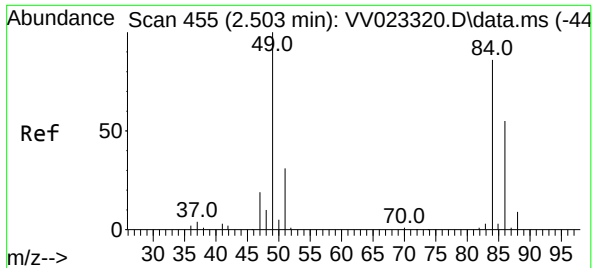

#16
Methylene chloride
Concen: 0.409 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV023328.D
Acq: 10 Nov 2021 13:22

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4408

Ion	Ratio	Lower	Upper
84	100		
86	58.3	42.3	78.5
49	114.5	79.7	148.1

