

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023329.D
 Acq On : 10 Nov 2021 13:45
 Operator : SY/MD
 Sample : M4492-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 11 00:41:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 11 00:38:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122377	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	125786	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57807	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36799	4.800	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.000%
7) Chloroethane-d5	1.568	69	29979	4.798	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.000%
11) 1,1-Dichloroethene-d2	2.108	63	51601	3.595	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.912	46	53405	40.434	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.860%
24) Chloroform-d	4.352	84	72473	4.436	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	5.037	65	34576	4.706	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	5.053	84	141074	4.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
36) 1,2-Dichloropropane-d6	6.072	67	41876	4.408	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	7.317	98	122248	4.042	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	7.625	79	14759	4.097	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.000%
46) 2-Hexanone-d5	8.091	63	41799	31.536	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	63.080%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27593	4.039	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	45948	4.774	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.400%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	4035	0.379	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023329.D
Acq On : 10 Nov 2021 13:45
Operator : SY/MD
Sample : M4492-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 11 00:41:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 11 00:38:57 2021
Response via : Initial Calibration

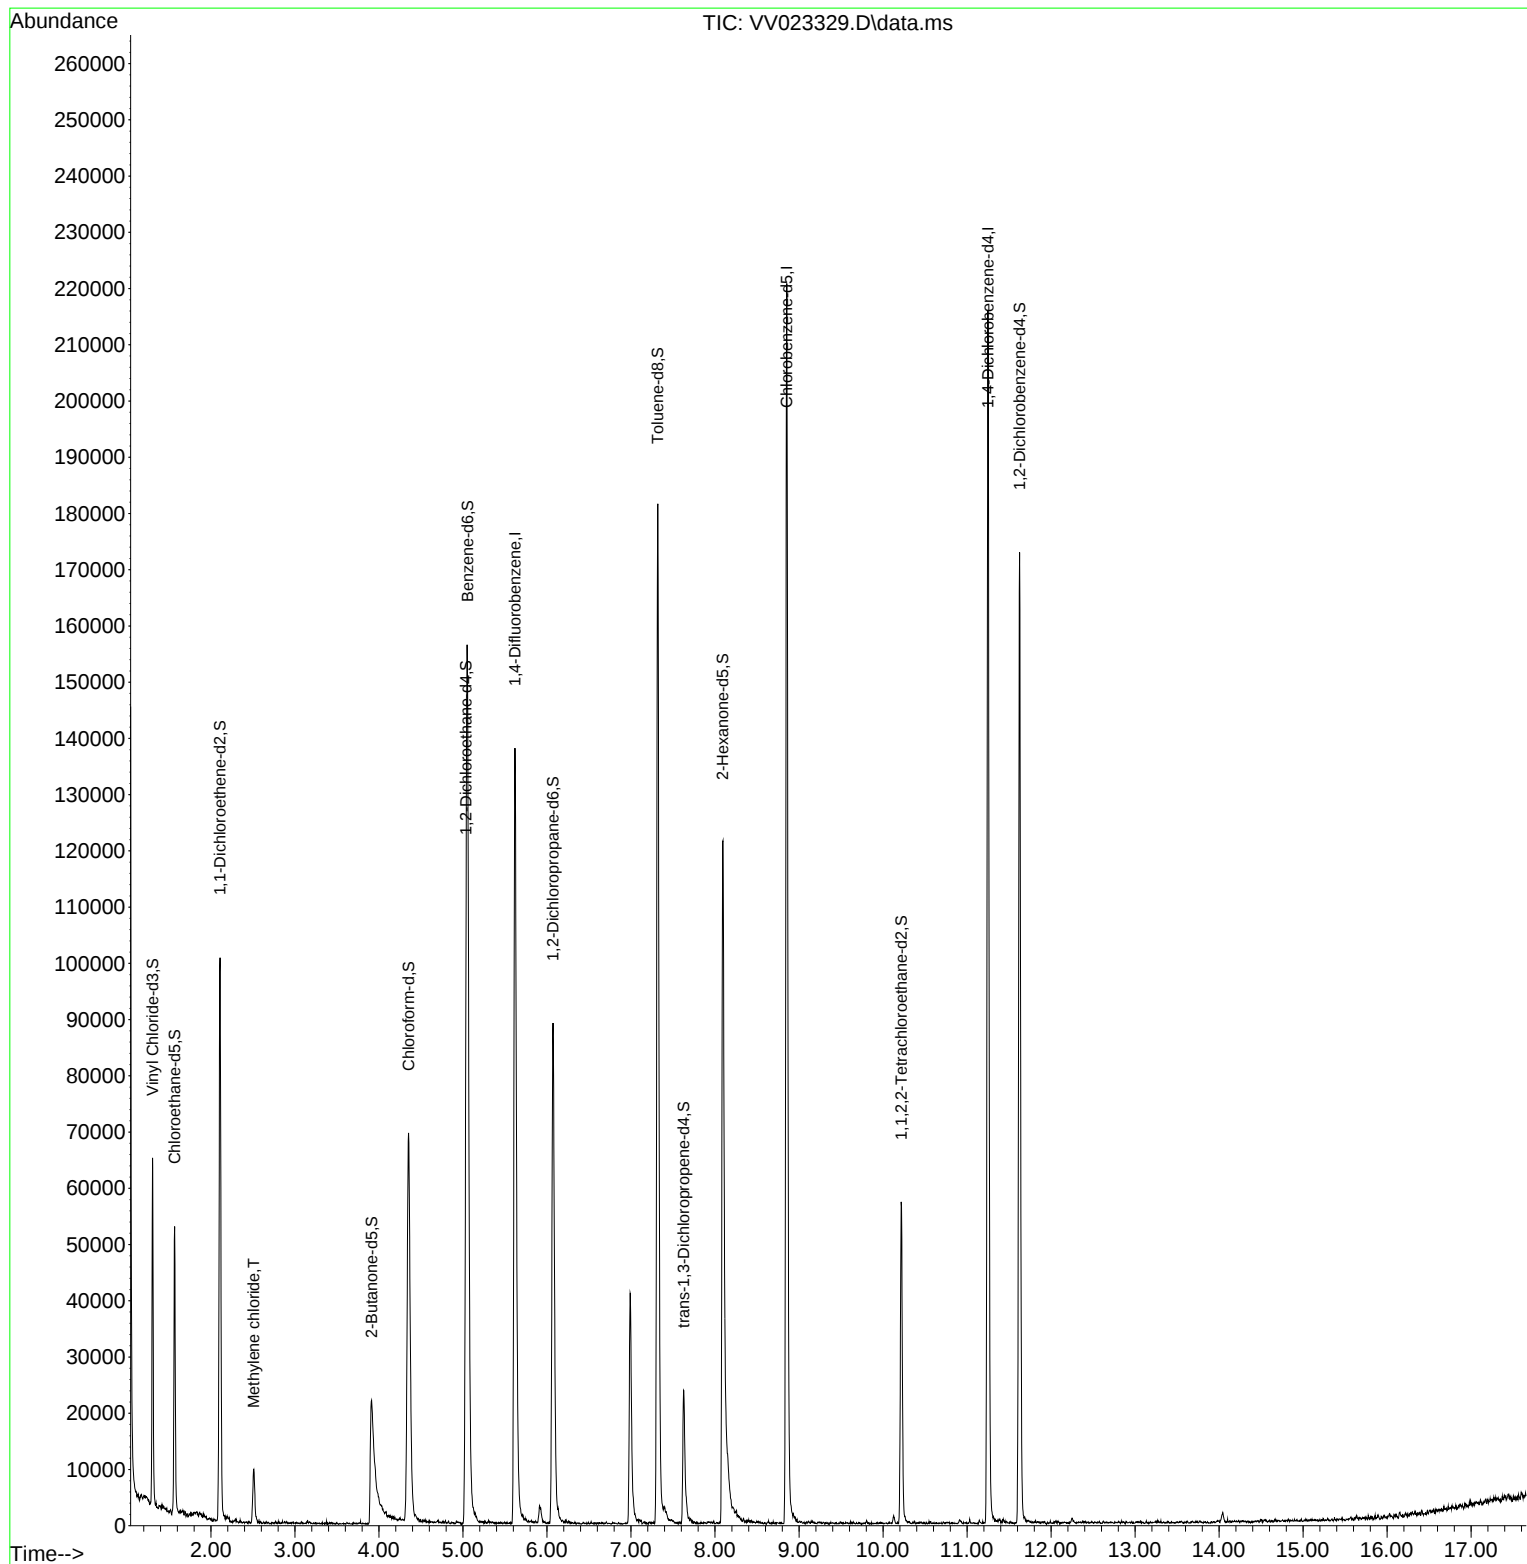

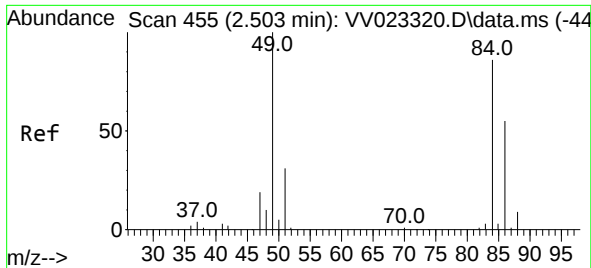

#16
Methylene chloride
Concen: 0.379 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV023329.D
Acq: 10 Nov 2021 13:45

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

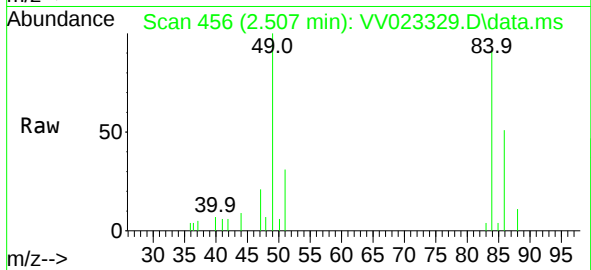

Tgt Ion: 84 Resp: 4035

Ion	Ratio	Lower	Upper
84	100		
86	56.7	42.3	78.5
49	110.3	79.7	148.1

